
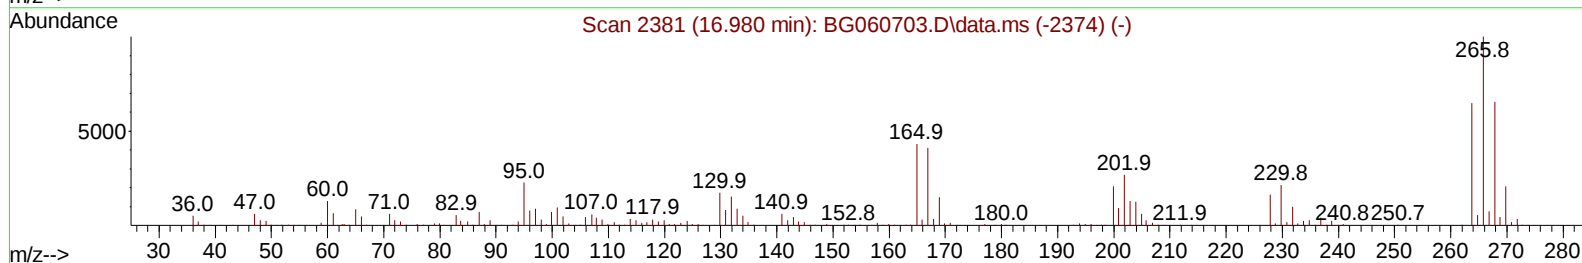
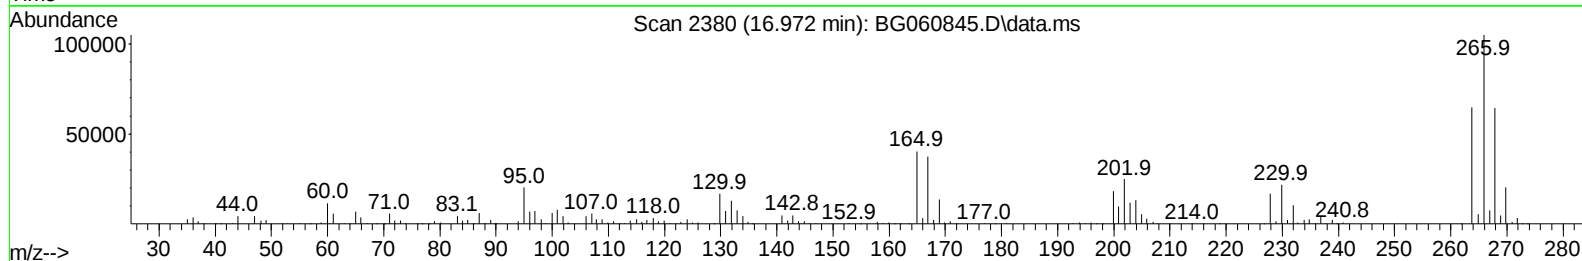


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041024\
Data File : BG060845.D
Acq On : 10 Apr 2024 8:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 11:02:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

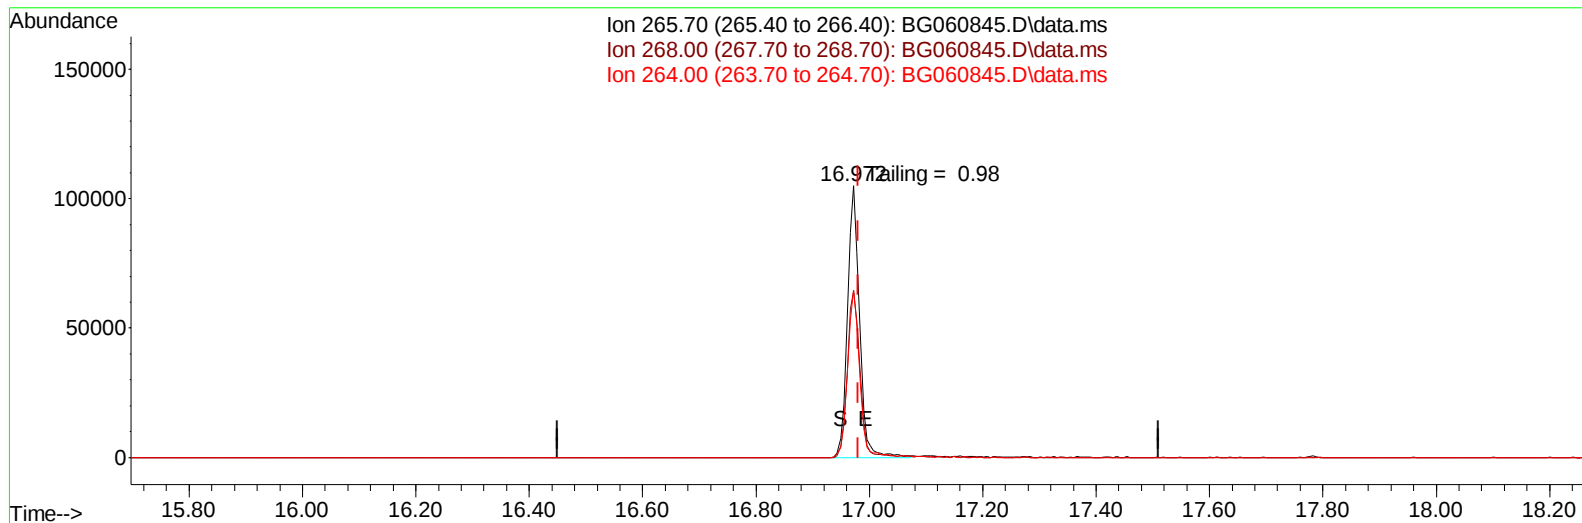




TIC: BG060845.D\data.ms

(70) Pentachlorophenol (C)**16.972min (-0.008) 293610.17 ng****response 155835**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	61.51
264.00	64.70	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041024\
Data File : BG060845.D
Acq On : 10 Apr 2024 8:55
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 11:02:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

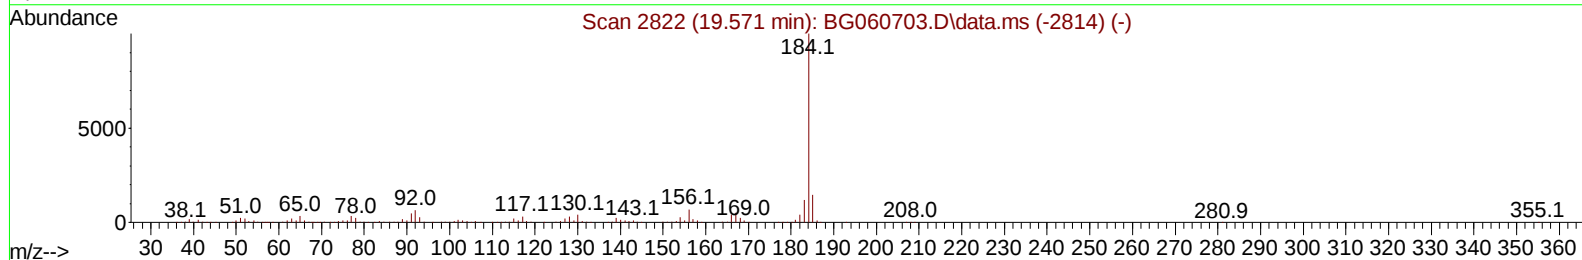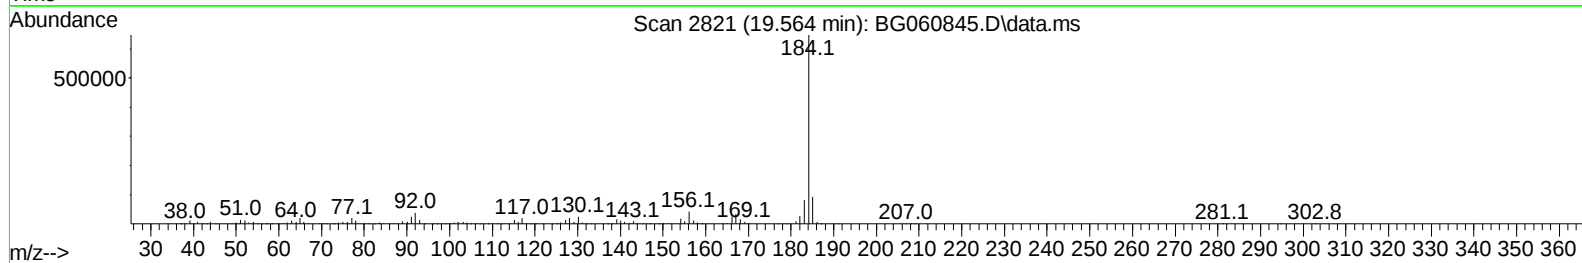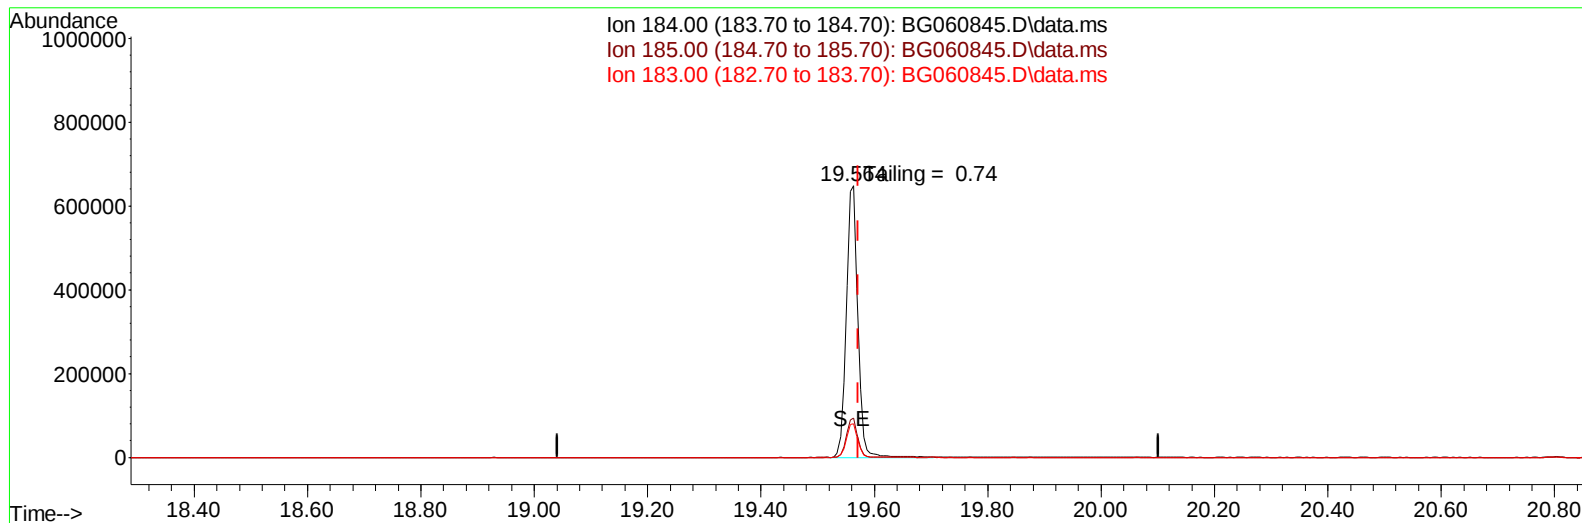

TIC: BG060845.D\data.ms

(77) Benzidine**19.564min (-0.008) 61543.50 ng****response 926968**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.42
183.00	11.90	12.42
0.00	0.00	0.00