

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041024\
 Data File : BG060852.D
 Acq On : 10 Apr 2024 16:31
 Operator : MA/JU
 Sample : P2022-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SU-03-04082024

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.094	12	18	19	rBV2	24629	35492	2.98%	0.508%
2	3.182	31	33	40	rVB3	12867	19101	1.60%	0.273%
3	5.533	427	433	442	rBV	95542	160157	13.43%	2.291%
4	7.107	694	701	711	rBV	105401	178502	14.97%	2.553%
5	7.947	837	844	851	rVB	304965	496142	41.60%	7.096%
6	9.099	1032	1040	1047	rBV	66206	112772	9.45%	1.613%
7	10.744	1313	1320	1329	rBV	379610	669393	56.12%	9.575%
8	13.200	1732	1738	1744	rBV	173641	258771	21.70%	3.701%
9	14.575	1965	1972	1979	rBV	615498	928403	77.84%	13.279%
10	16.061	2219	2225	2233	rBV	119236	191390	16.05%	2.738%
11	16.326	2264	2270	2279	rVB	4984	14393	1.21%	0.206%
12	17.101	2398	2402	2407	rBV8	8003	12314	1.03%	0.176%
13	17.319	2433	2439	2445	rBV	763145	1148067	96.25%	16.421%
14	17.360	2445	2446	2452	rVB	27873	29833	2.50%	0.427%
15	18.229	2590	2594	2601	rVB9	17488	34224	2.87%	0.490%
16	19.375	2786	2789	2794	rVB	46760	57702	4.84%	0.825%
17	19.739	2847	2851	2856	rVB2	79655	116905	9.80%	1.672%
18	19.945	2881	2886	2890	rBV	293620	386599	32.41%	5.530%
19	21.584	3159	3165	3172	rVB	740590	1192739	100.00%	17.060%
20	24.722	3693	3699	3707	rVB	361822	948500	79.52%	13.567%




Sum of corrected areas: 6991399

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041024\
Data File : BG060852.D
Acq On : 10 Apr 2024 16:31
Operator : MA/JU
Sample : P2022-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SU-03-04082024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

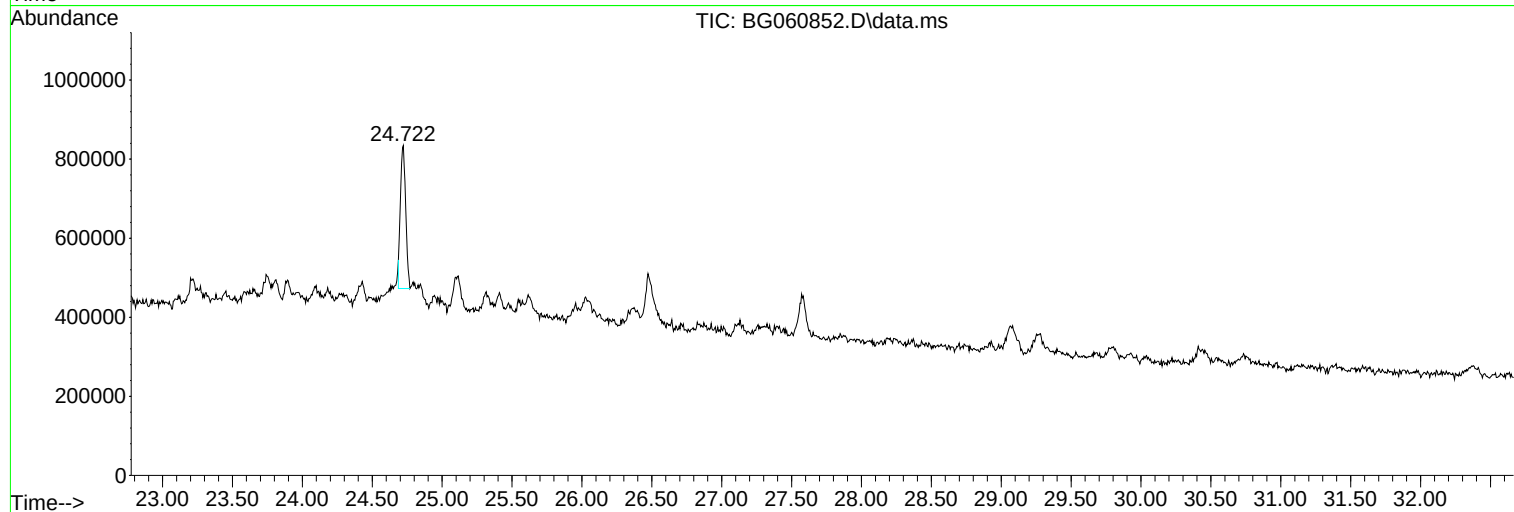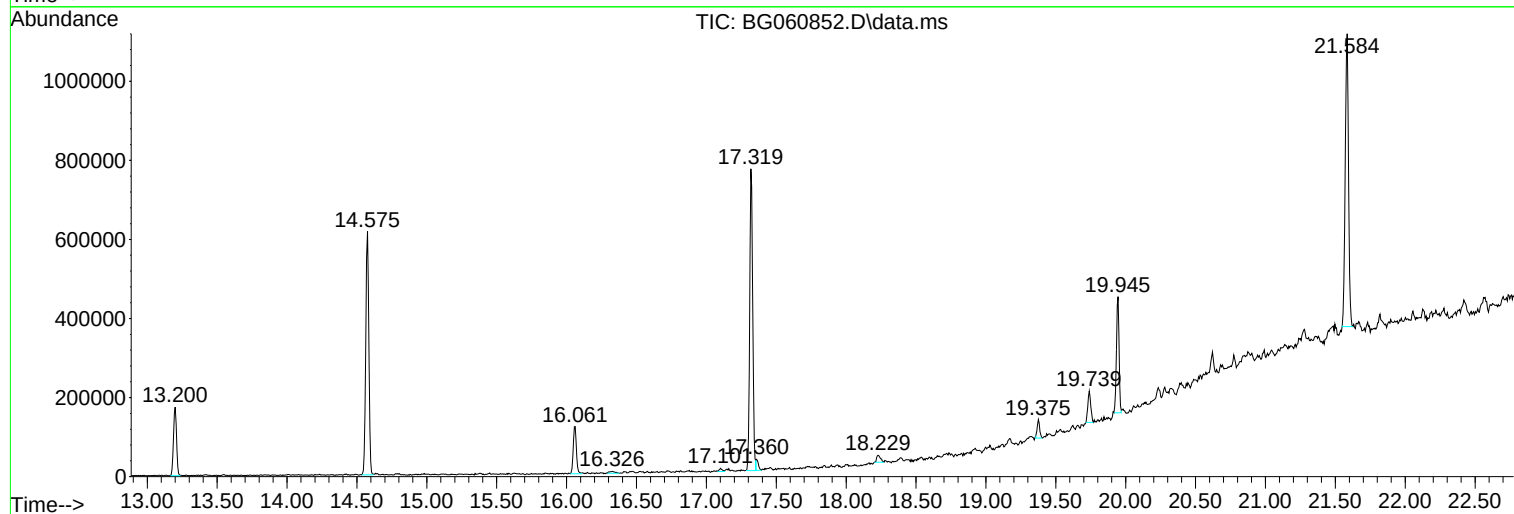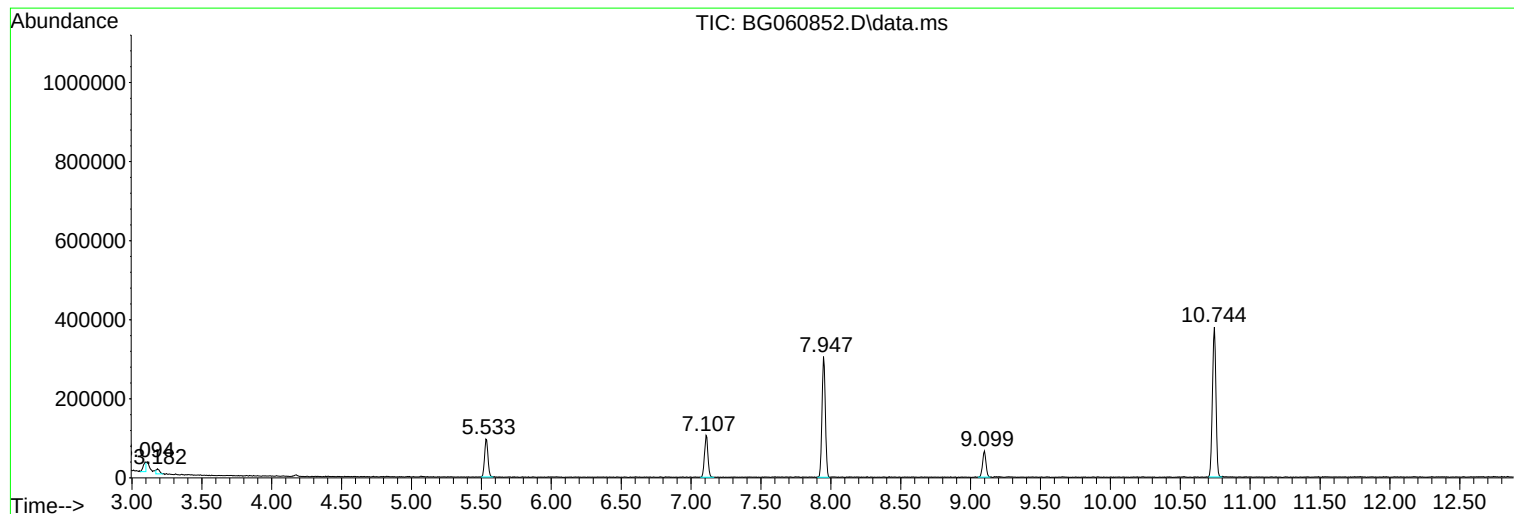

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041024\
Data File : BG060852.D
Acq On : 10 Apr 2024 16:31
Operator : MA/JU
Sample : P2022-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SU-03-04082024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041024\
Data File : BG060852.D
Acq On : 10 Apr 2024 16:31
Operator : MA/JU
Sample : P2022-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SU-03-04082024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------