


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041024\
Data File : BG060845.D
Acq On : 10 Apr 2024 8:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

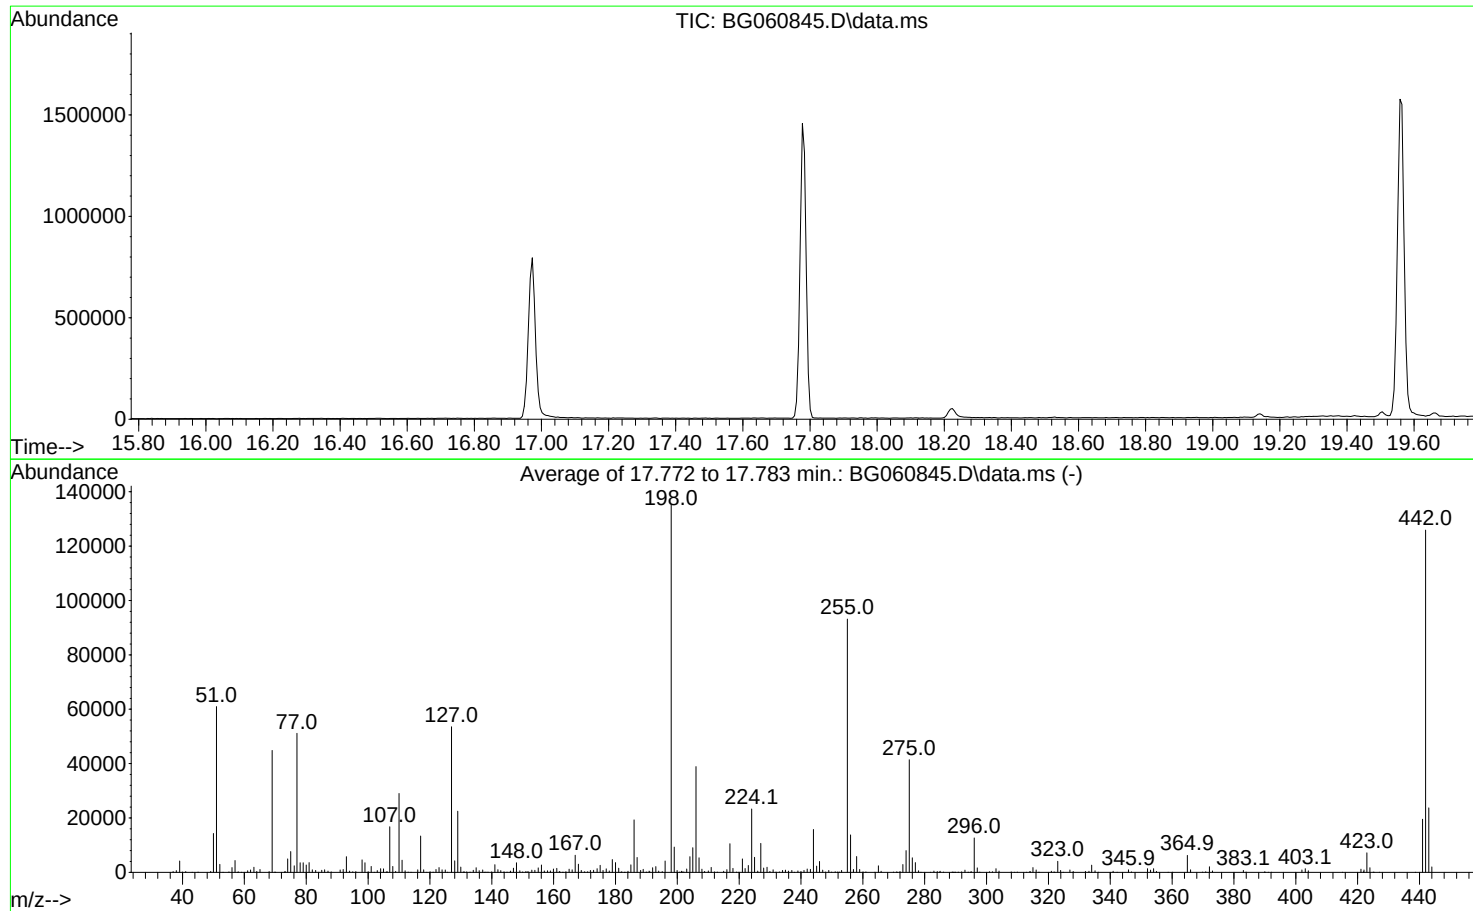




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	60949	PASS
68	69	0.00	2	0.6	279	PASS
69	198	0.00	100	33.1	44837	PASS
70	69	0.00	2	0.3	150	PASS
127	198	10	80	39.6	53565	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	135301	PASS
199	198	5	9	6.9	9289	PASS
275	198	10	60	30.6	41421	PASS
365	198	1	100	4.6	6255	PASS
441	198	0.01	100	14.5	19554	PASS
442	442	50	100	100.0	125869	PASS
443	442	15	24	18.8	23712	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041024\
Data File : BG060845.D
Acq On : 10 Apr 2024 8:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 10 11:02:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

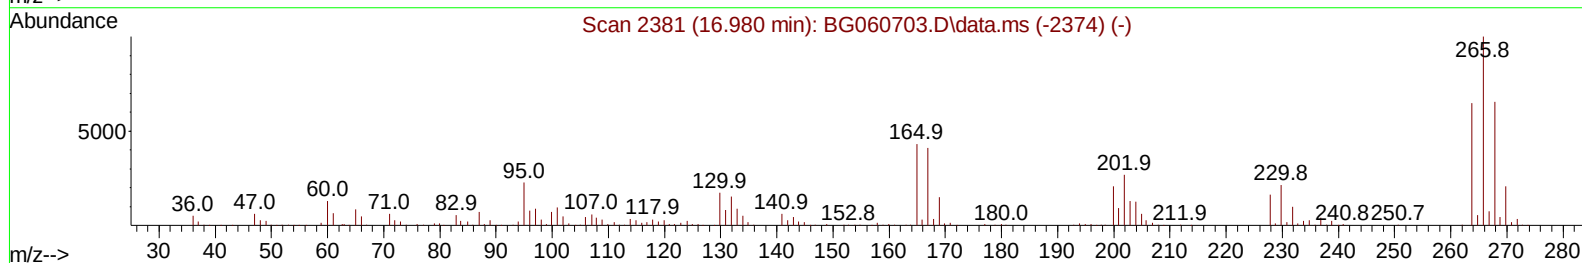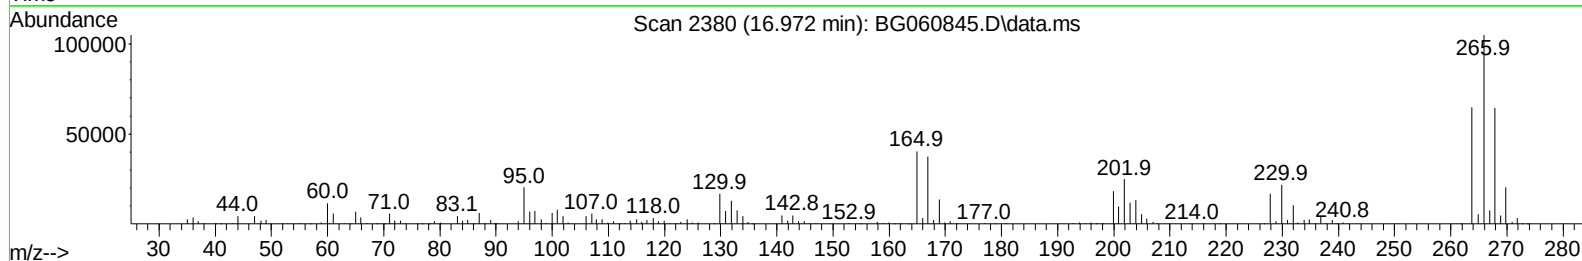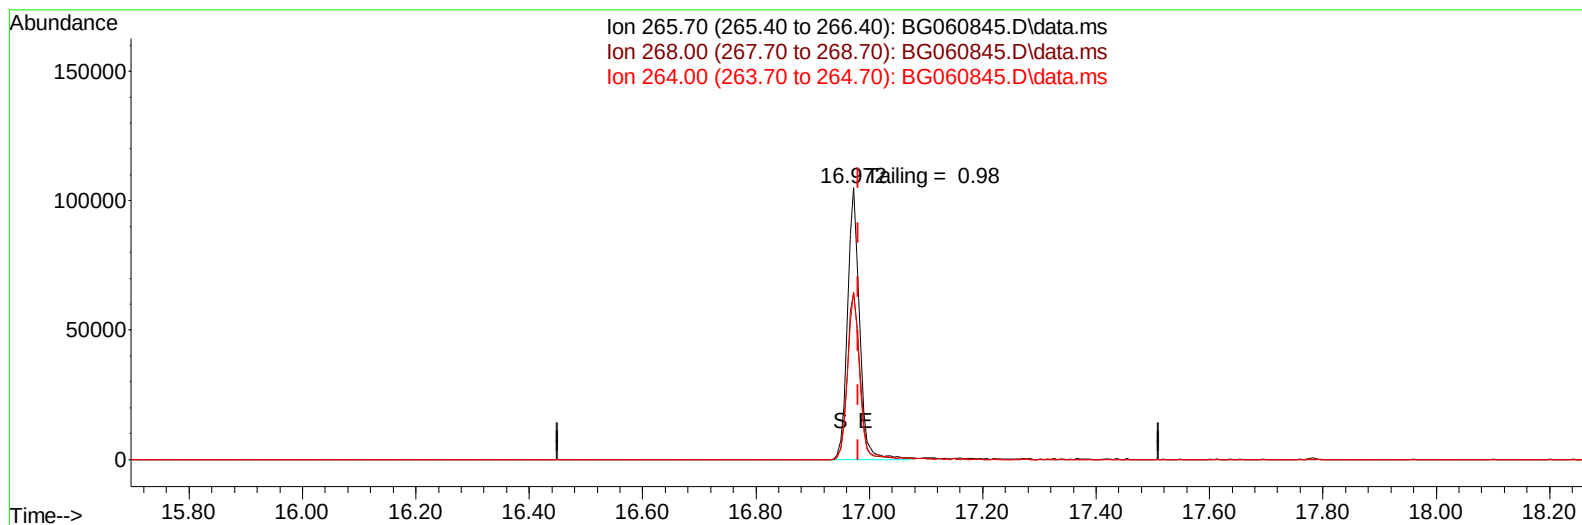

TIC: BG060845.D\data.ms

(70) Pentachlorophenol (C)

16.972min (-0.008) 293610.17 ng




response 155835

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	61.51
264.00	64.70	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041024\
Data File : BG060845.D
Acq On : 10 Apr 2024 8:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 10 11:02:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

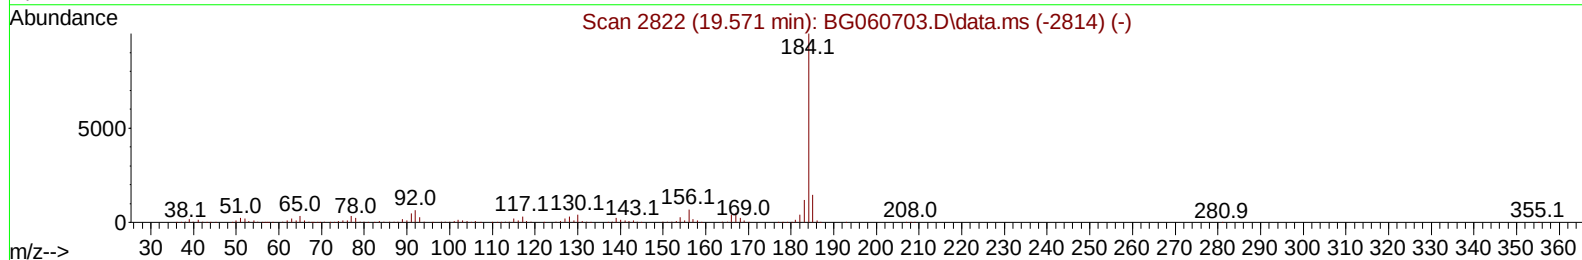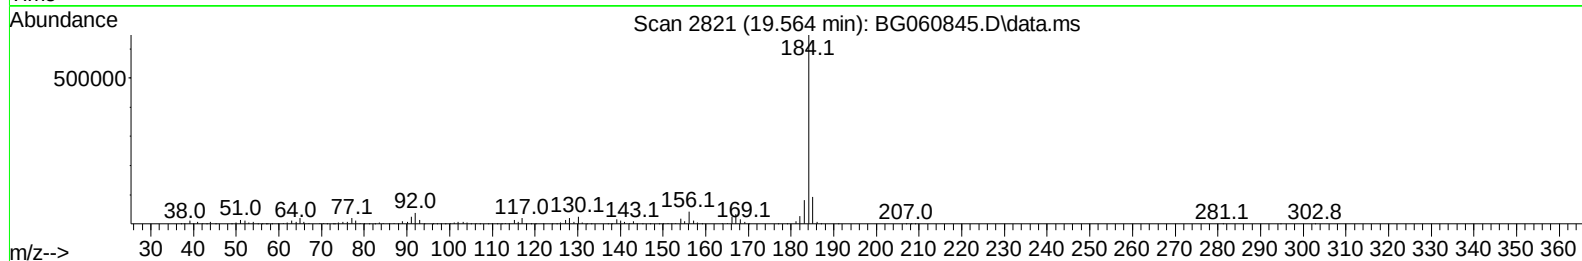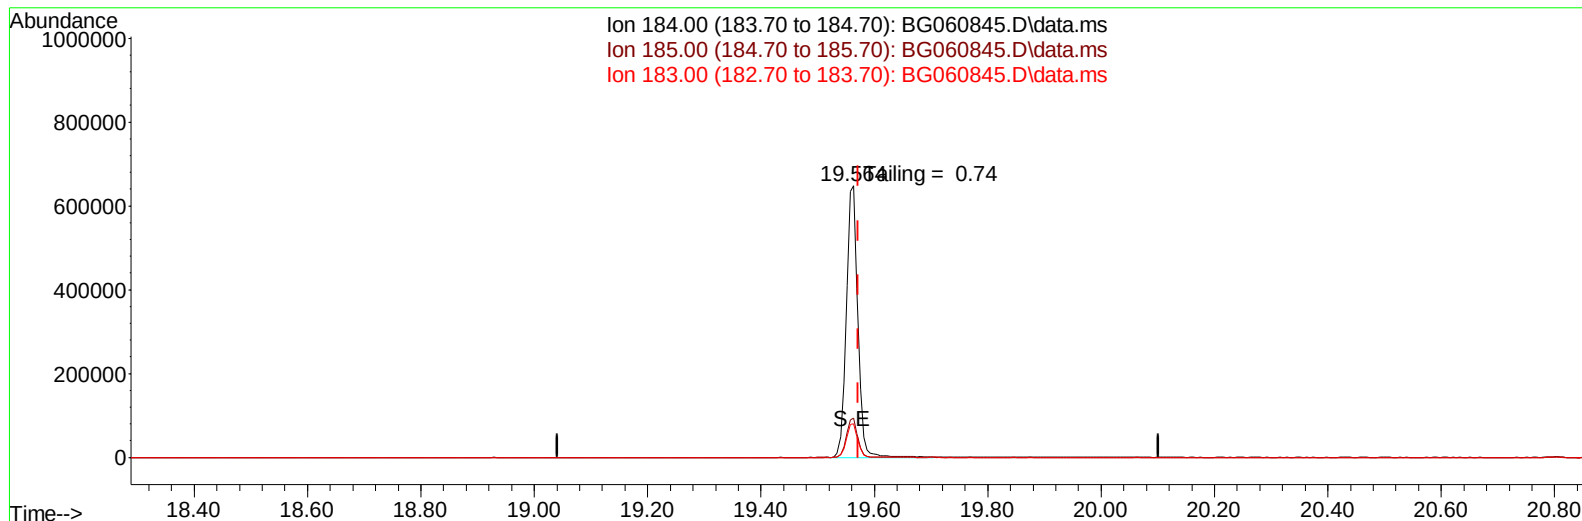

TIC: BG060845.D\data.ms

(77) Benzidine

19.564min (-0.008) 61543.50 ng

response 926968

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.42
183.00	11.90	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/10/2024	BNA_G	<u>BG060845.D</u>
Compound Name	Response	Retention Time
DDT	464565	20.803
DDD	11699	20.363
DDE	3000	19.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14699	479264	3.07

Instrument :
BNA_G
ClientSampleId :
DFTPP