
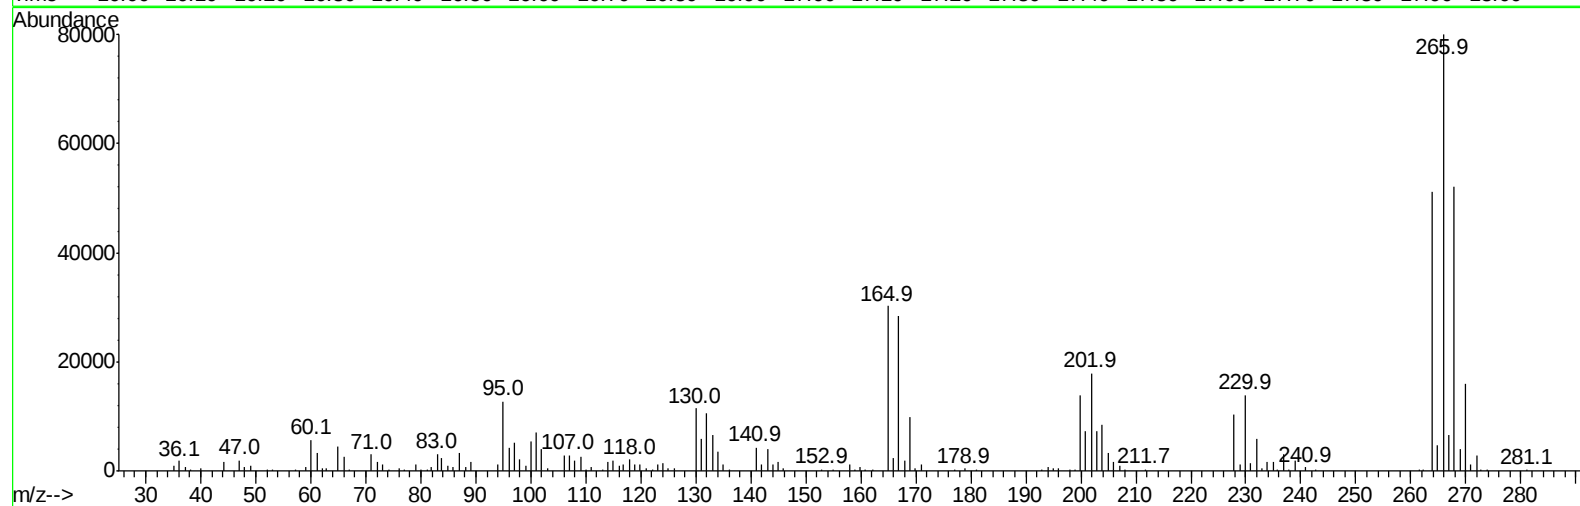


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041117\
Data File : BG026618.D
Acq On : 11 Apr 2017 15:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 09:35:52 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

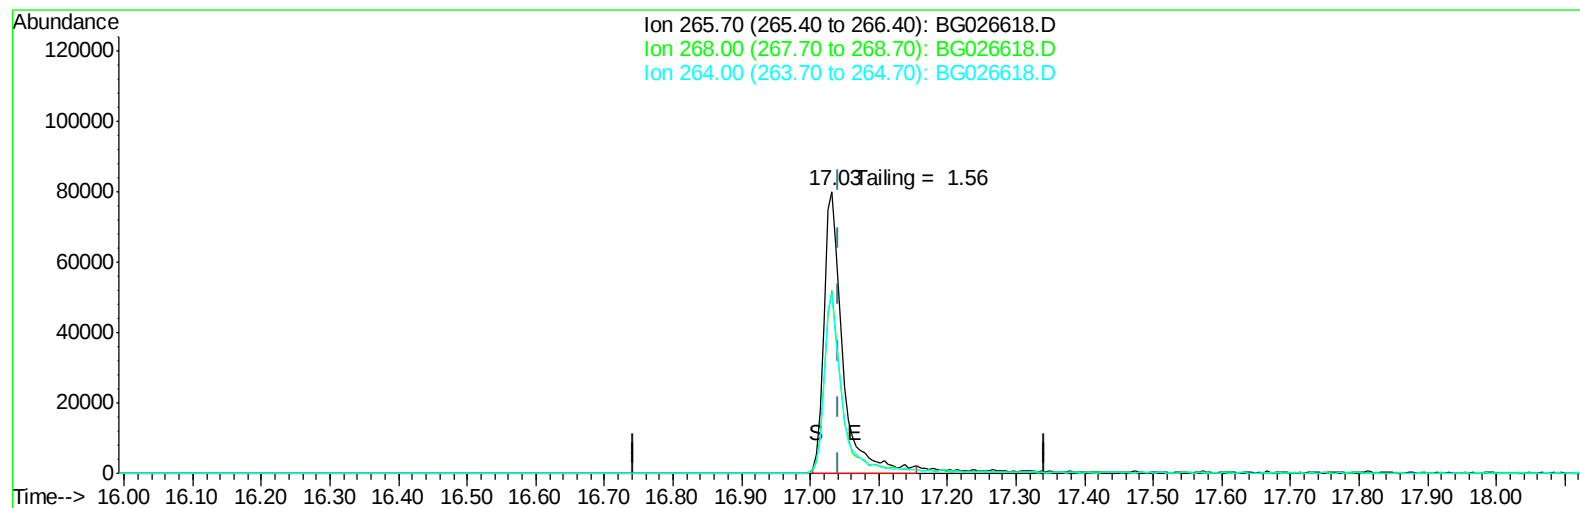

TIC: BG026618.D

(69) Pentachlorophenol (C)



17.032min (-0.011) 0.00ng

response 149085

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	65.16
264.00	62.60	63.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041117\
Data File : BG026618.D
Acq On : 11 Apr 2017 15:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 09:35:52 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

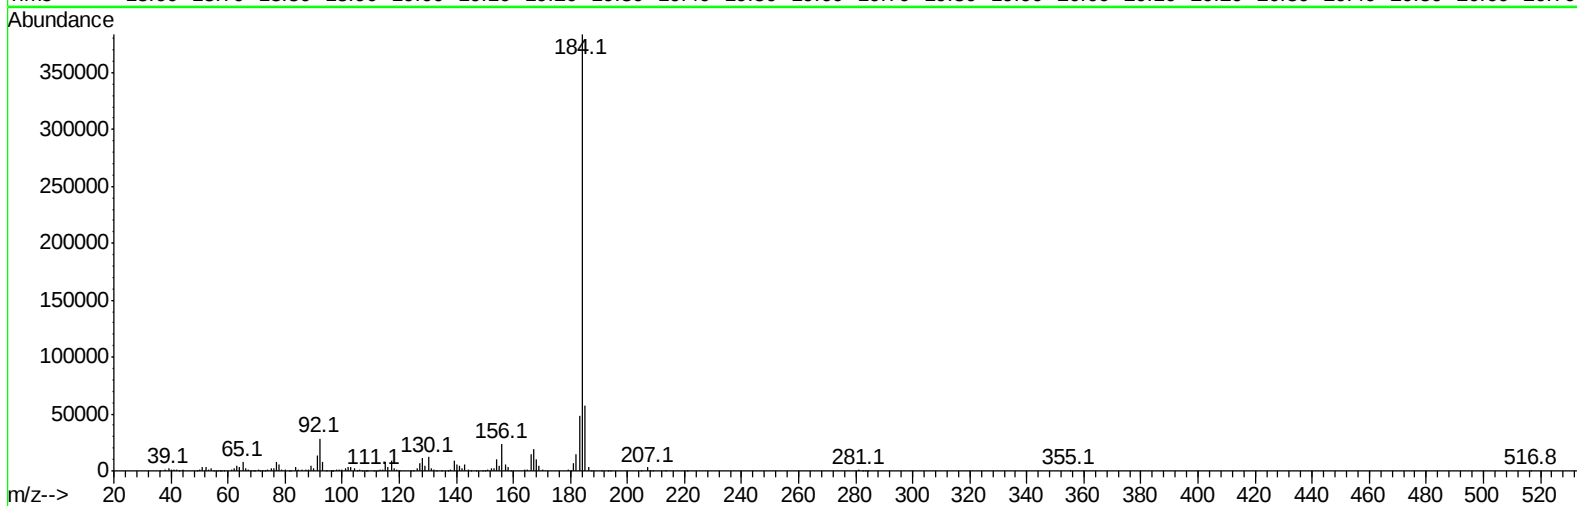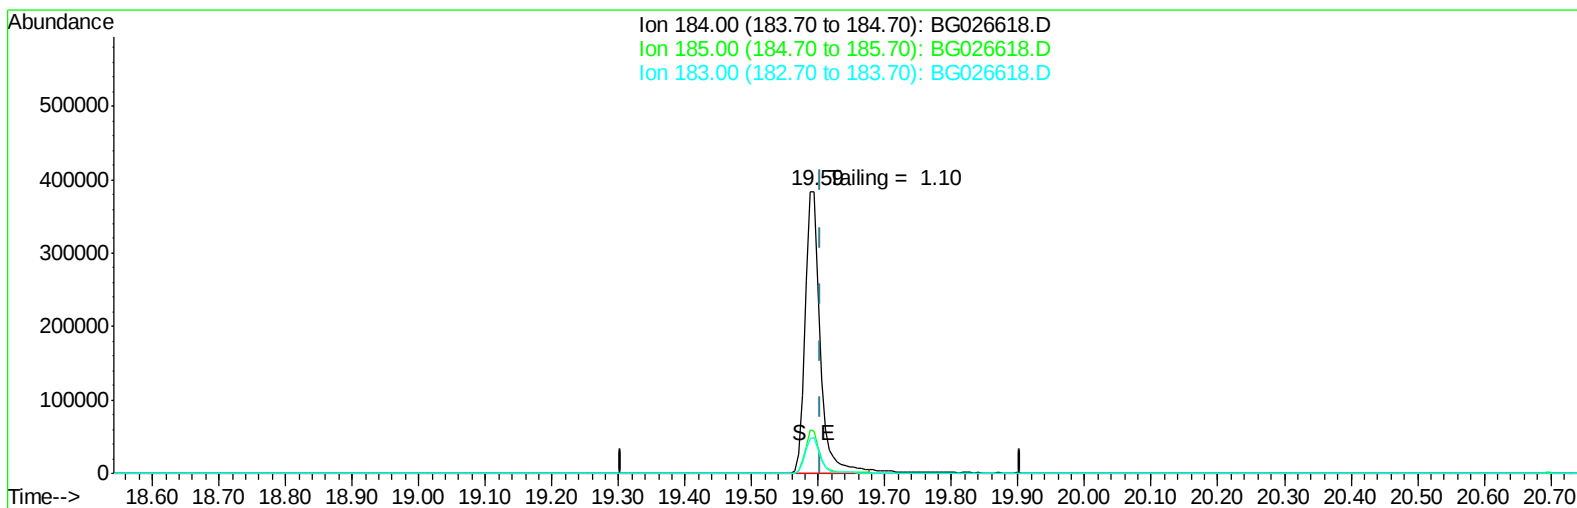

TIC: BG026618.D

(76) Benzidine

19.594min (-0.011) 139096.63ng m

response 613866

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.89
183.00	13.80	12.72
0.00	0.00	0.00