


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041117\
 Data File : BG026618.D
 Acq On : 11 Apr 2017 15:07
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 20 17:43:27 2017

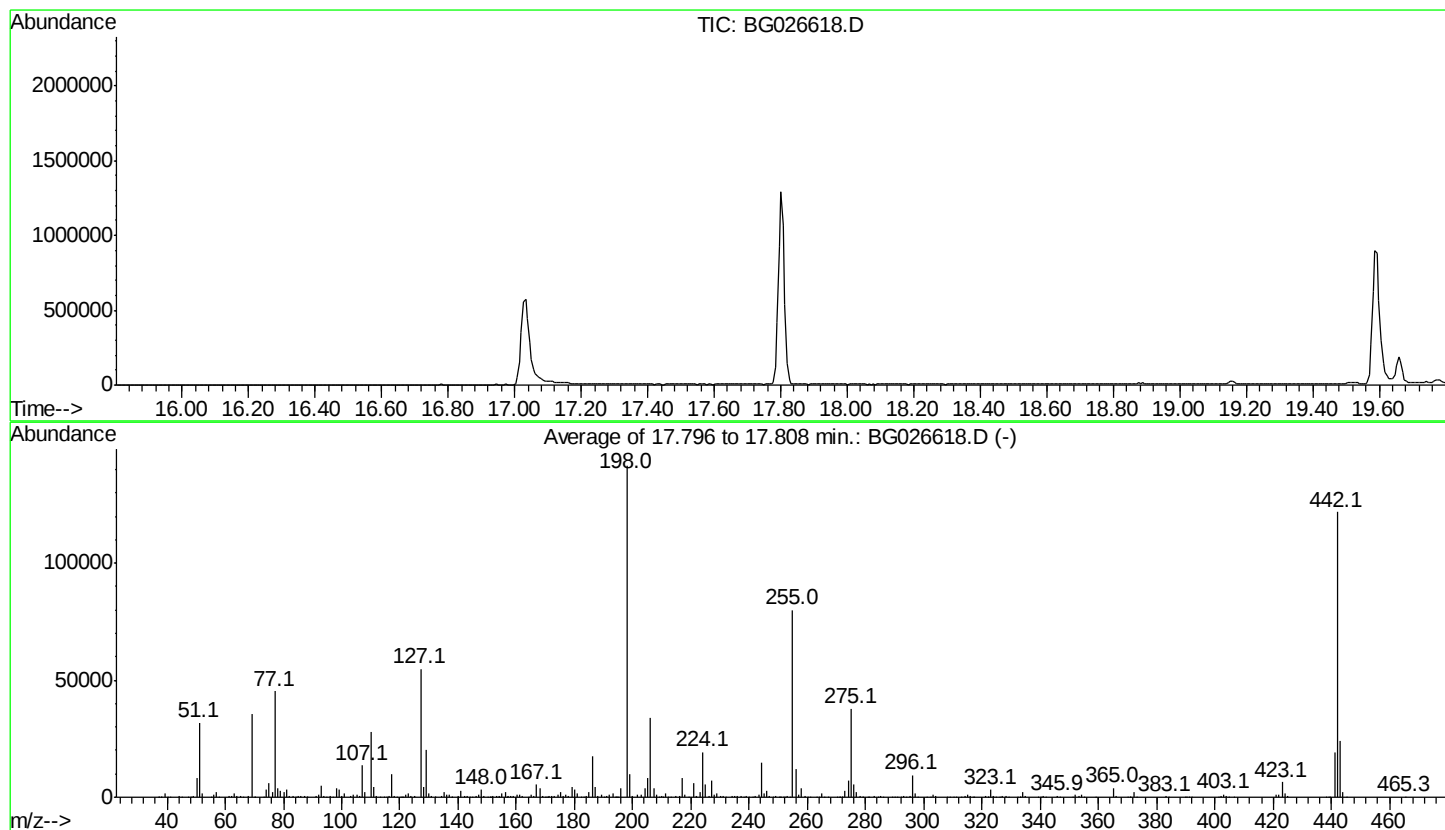

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	31792	PASS
68	69	0.00	2	0.9	314	PASS
69	198	0.00	100	25.2	35698	PASS
70	69	0.00	2	0.7	260	PASS
127	198	10	80	38.8	54917	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	141629	PASS
199	198	5	9	6.9	9828	PASS
275	198	10	60	26.7	37773	PASS
365	198	1	100	2.9	4079	PASS
441	442	0.01	24	15.9	19378	PASS
442	198	50	100	86.0	121760	PASS
443	442	15	24	19.7	24013	PASS