
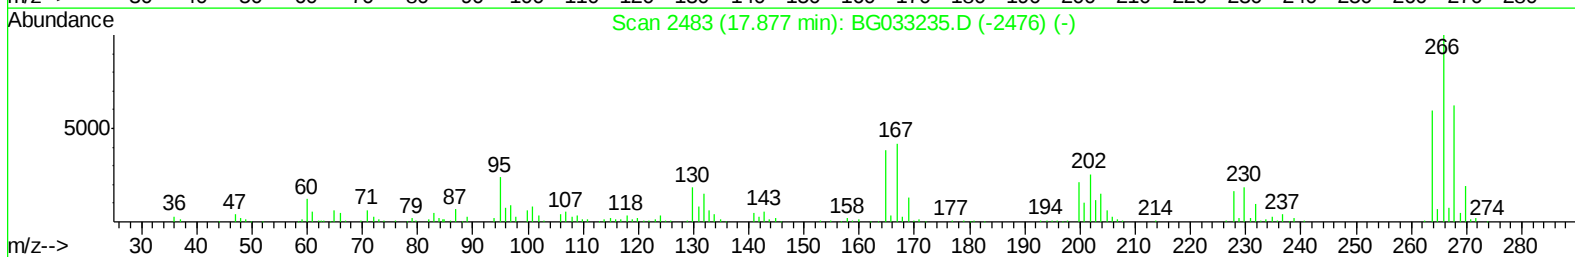
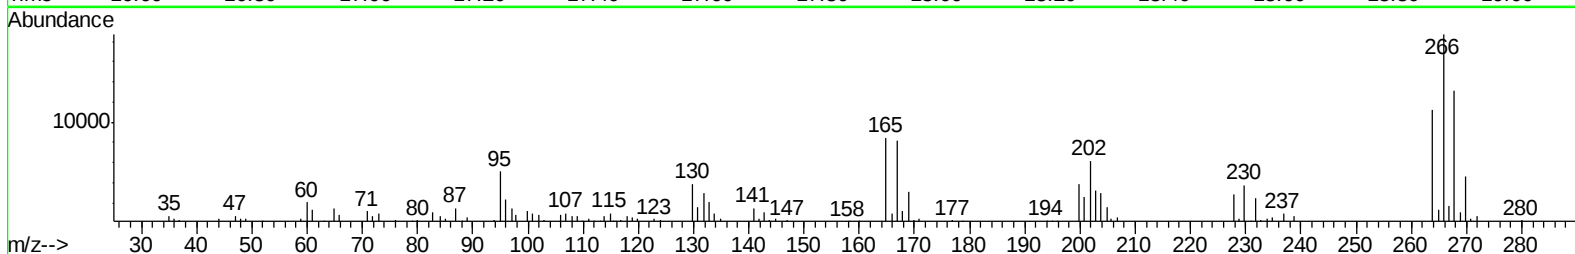


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041118\
 Data File : BG033746.D
 Acq On : 11 Apr 2018 15:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Apr 12 07:43:30 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 10 16:51:36 2018
 Response via : Initial Calibration

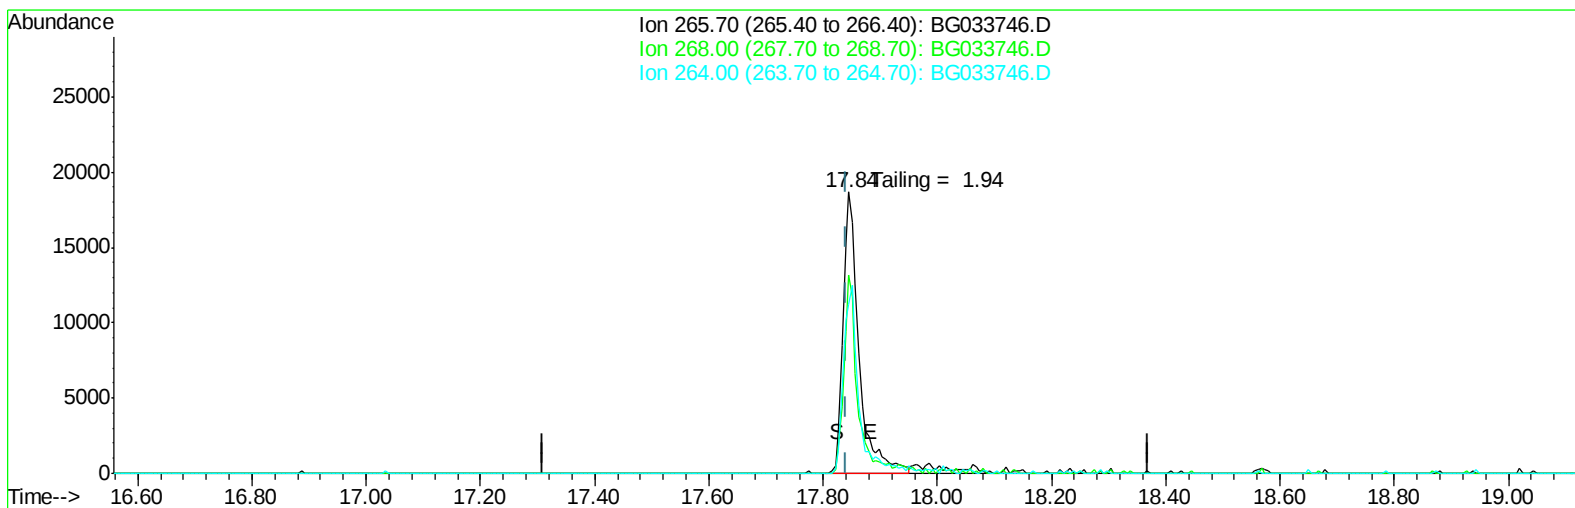

TIC: BG033746.D

(69) Pentachlorophenol (C)

17.845min (+0.004) 12788.62ng

response 36445

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	70.29
264.00	62.00	60.03
0.00	0.00	0.00