
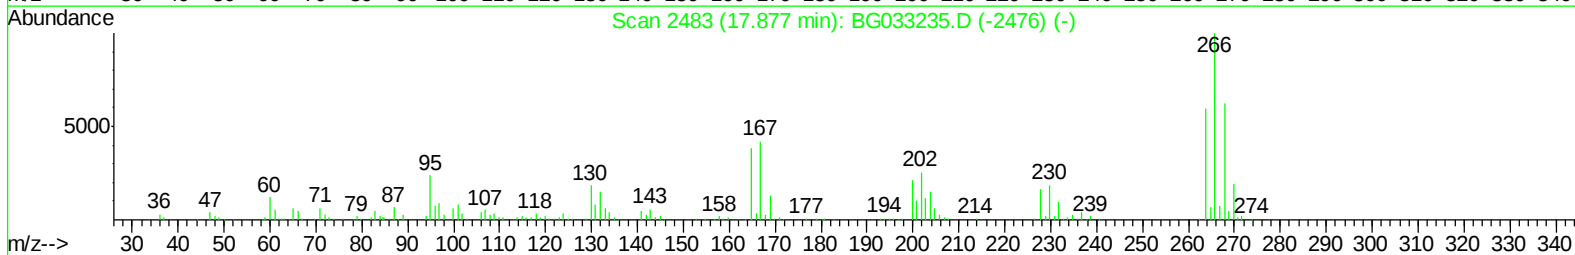
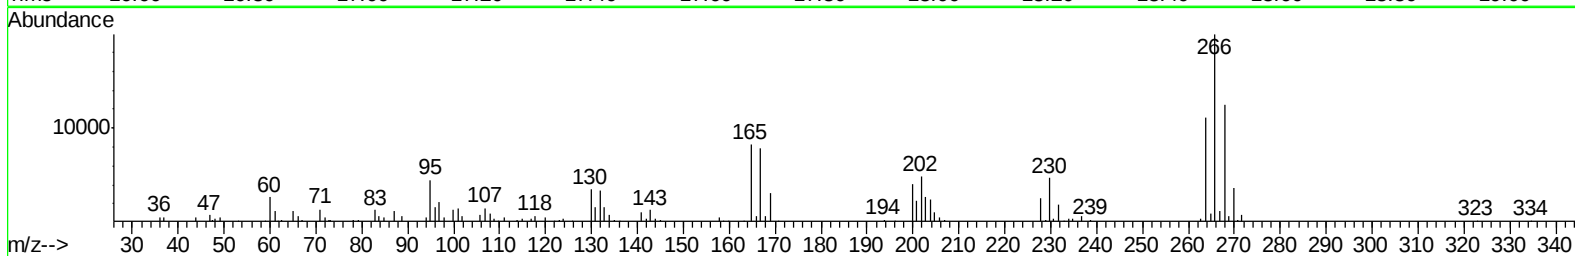


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041118\
Data File : BG033764.D
Acq On : 12 Apr 2018 3:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 07:45:35 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 16:51:36 2018
Response via : Initial Calibration

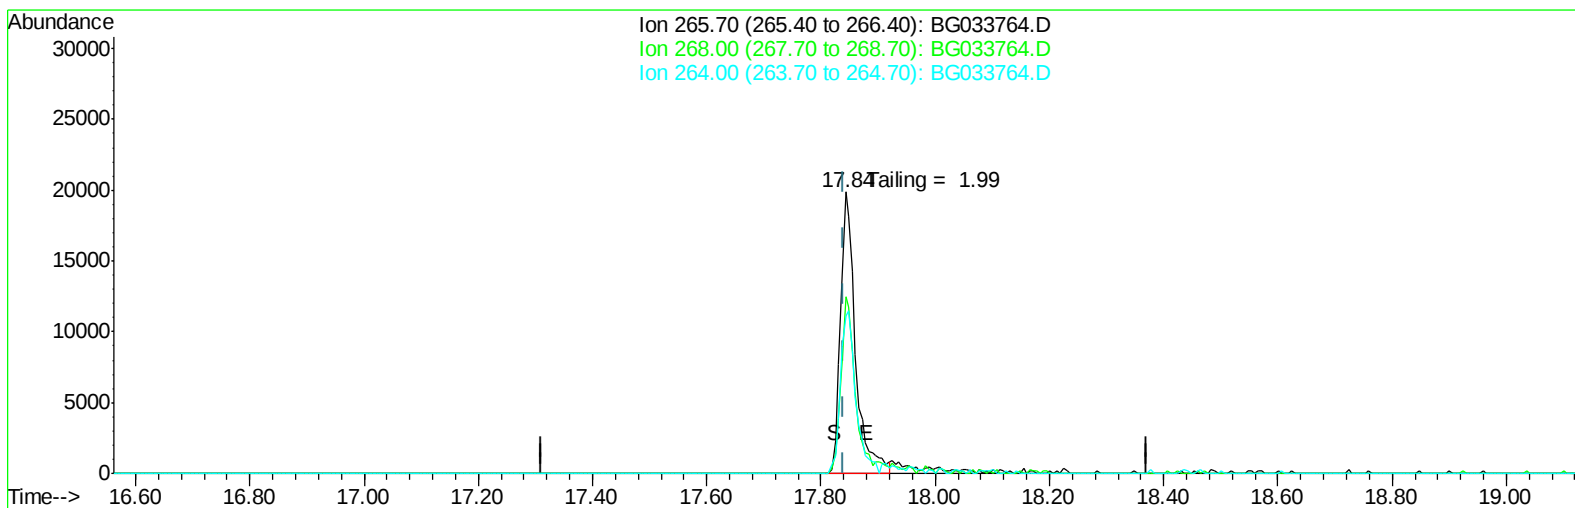

TIC: BG033764.D

(69) Pentachlorophenol (C)




17.843min (+0.002) 13643.54ng

response 36444

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.33
264.00	62.00	56.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041118\
 Data File : BG033764.D
 Acq On : 12 Apr 2018 3:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 07:45:35 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 10 16:51:36 2018
 Response via : Initial Calibration

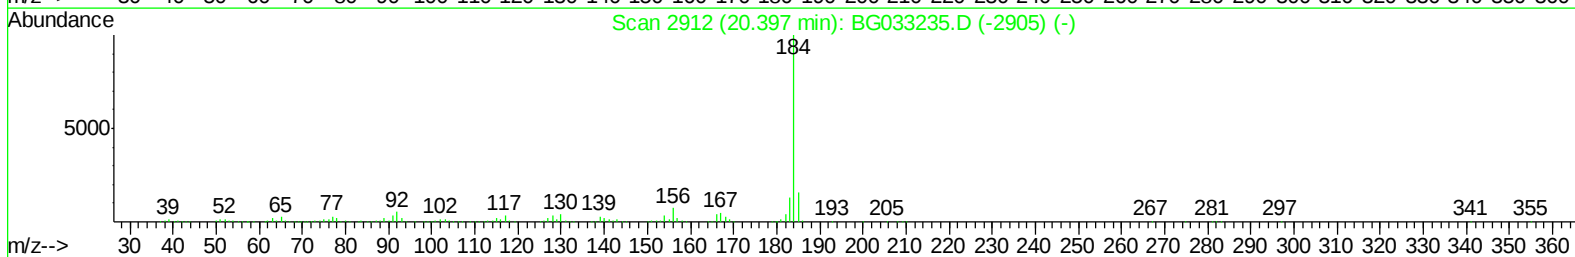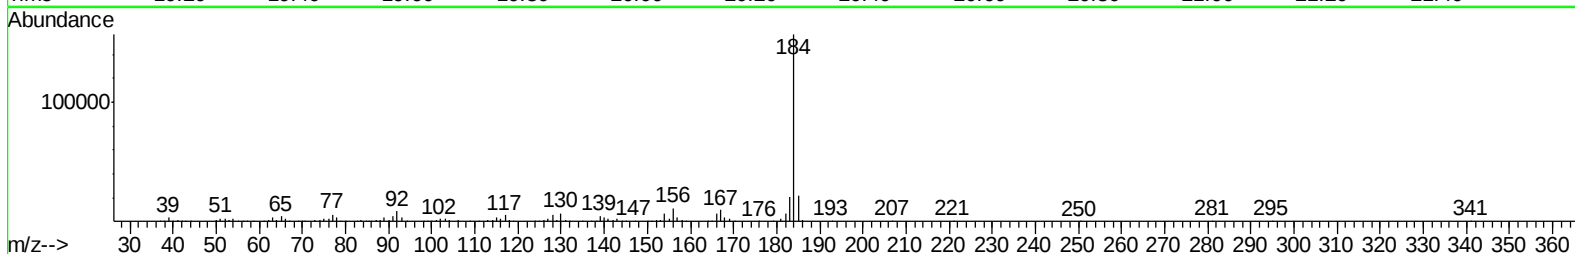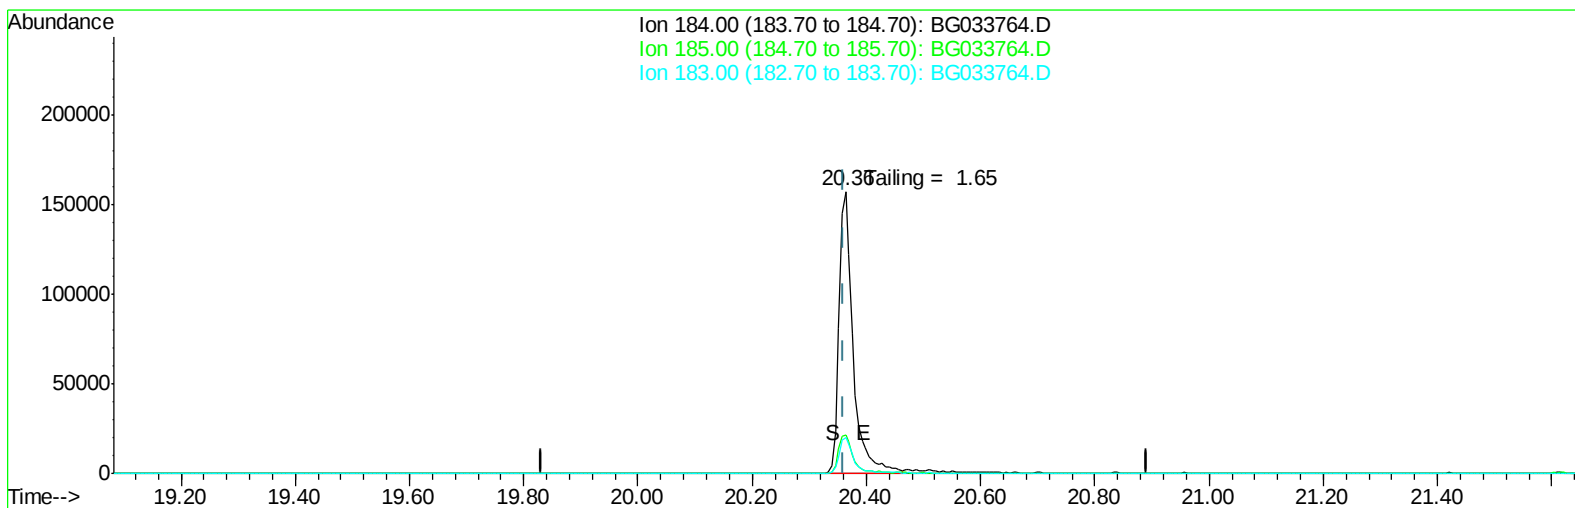

TIC: BG033764.D

(76) Benzidine

20.363min (+0.002) 122428.27ng

response 268926

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.79
183.00	13.30	12.96
0.00	0.00	0.00