


Data Path : Z:\HPCHEM1\BNA G\Data\BG041118\
 Data File : BG033746.D
 Acq On : 11 Apr 2018 15:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 10 16:51:36 2018

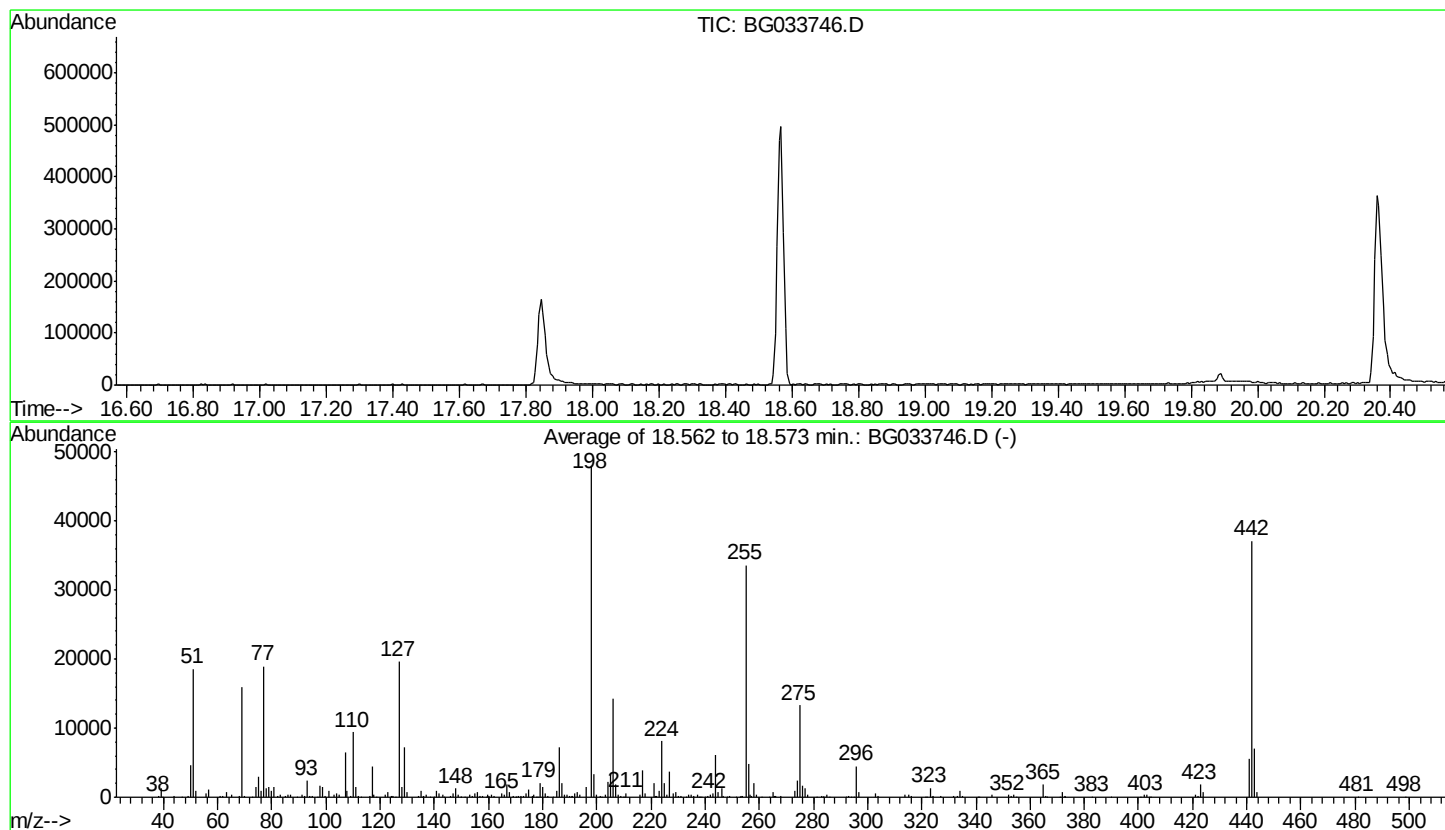

AutoFind: Scans 2599, 2600, 2601; Background Corrected with Scan 2592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	18553	PASS
68	69	0.00	2	1.6	249	PASS
69	198	0.00	100	33.4	16014	PASS
70	69	0.00	2	1.1	171	PASS
127	198	10	80	40.8	19571	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47989	PASS
199	198	5	9	6.9	3310	PASS
275	198	10	60	27.7	13311	PASS
365	198	1	100	3.8	1800	PASS
441	443	0.01	100	79.3	5586	PASS
442	198	50	100	77.4	37149	PASS
443	442	15	24	19.0	7046	PASS