


Data Path : Z:\HPCHEM1\BNA G\Data\BG041118\  
 Data File : BG033764.D  
 Acq On : 12 Apr 2018 3:33  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG031918.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Apr 10 16:51:36 2018

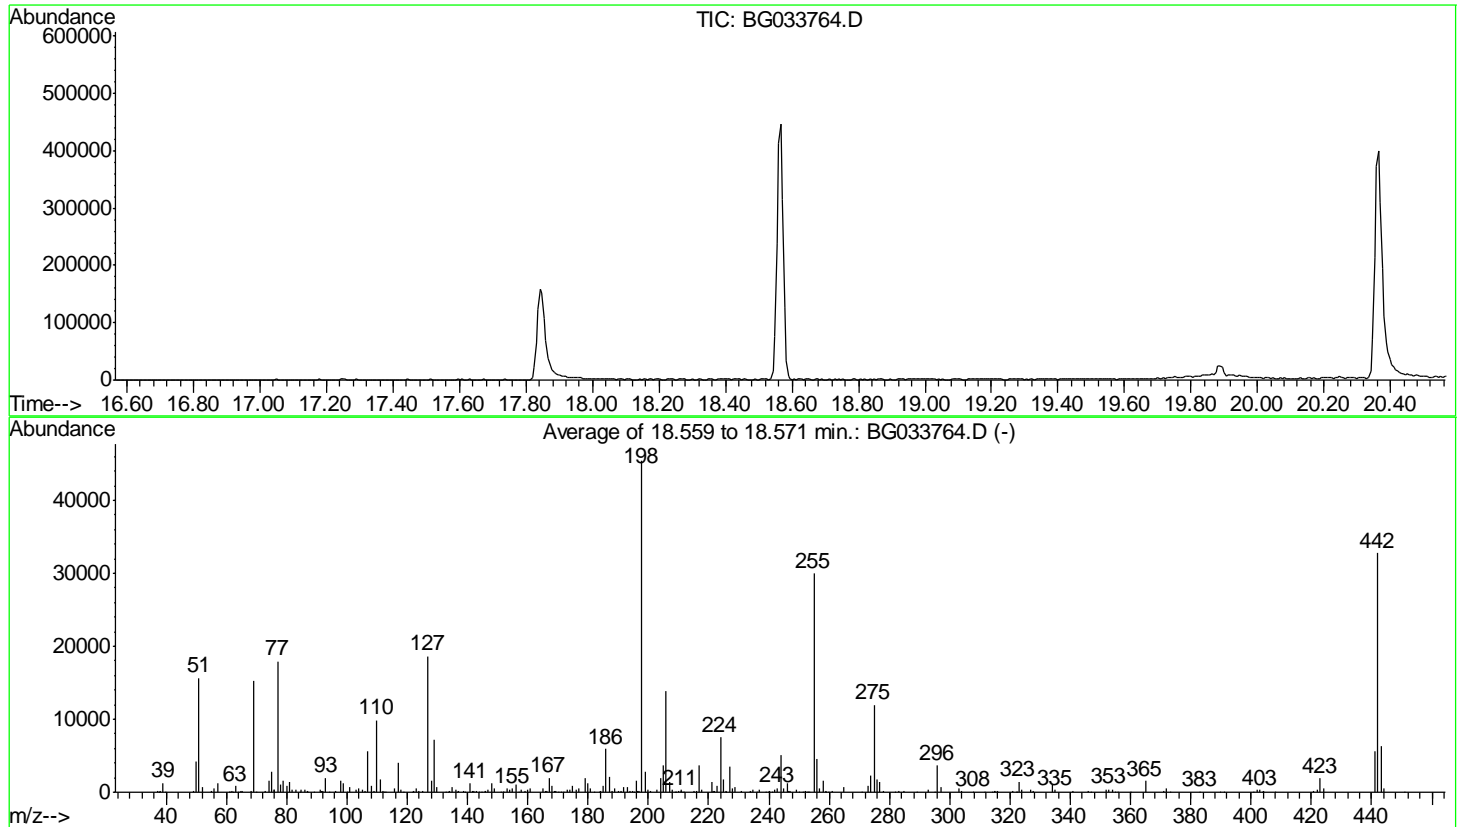

AutoFind: Scans 2599, 2600, 2601; Background Corrected with Scan 2592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	15660	PASS
68	69	0.00	2	1.7	254	PASS
69	198	0.00	100	33.8	15347	PASS
70	69	0.00	2	0.5	70	PASS
127	198	10	80	41.0	18607	PASS
197	198	0.00	2	0.4	189	PASS
198	198	100	100	100.0	45437	PASS
199	198	5	9	6.4	2887	PASS
275	198	10	60	26.4	11990	PASS
365	198	1	100	3.4	1545	PASS
441	443	0.01	100	87.9	5566	PASS
442	198	50	100	72.1	32768	PASS
443	442	15	24	19.3	6330	PASS