
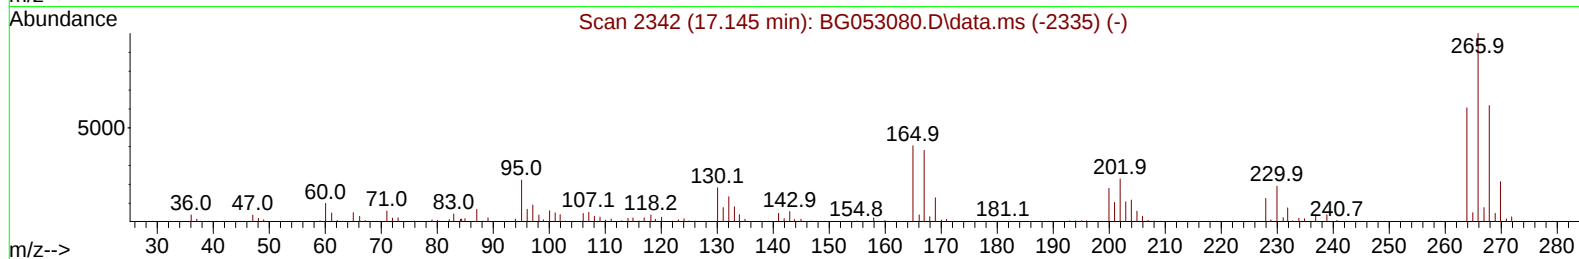
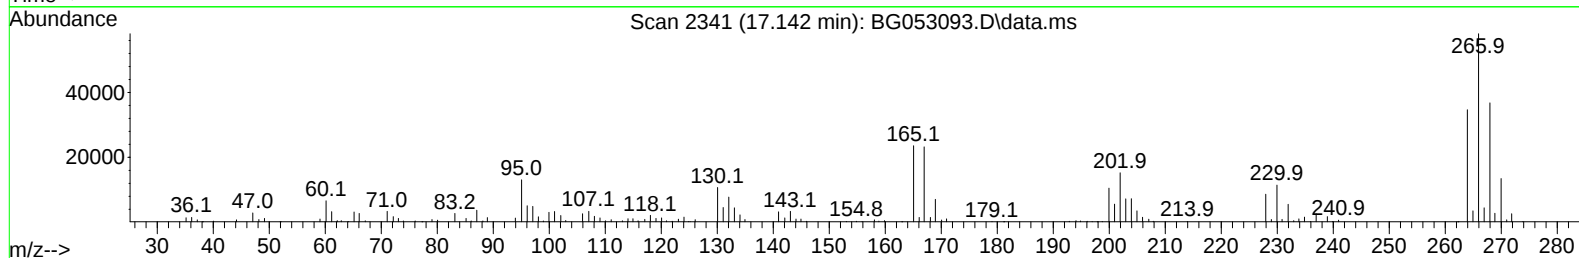


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041122\
Data File : BG053093.D
Acq On : 11 Apr 2022 9:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 08:19:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

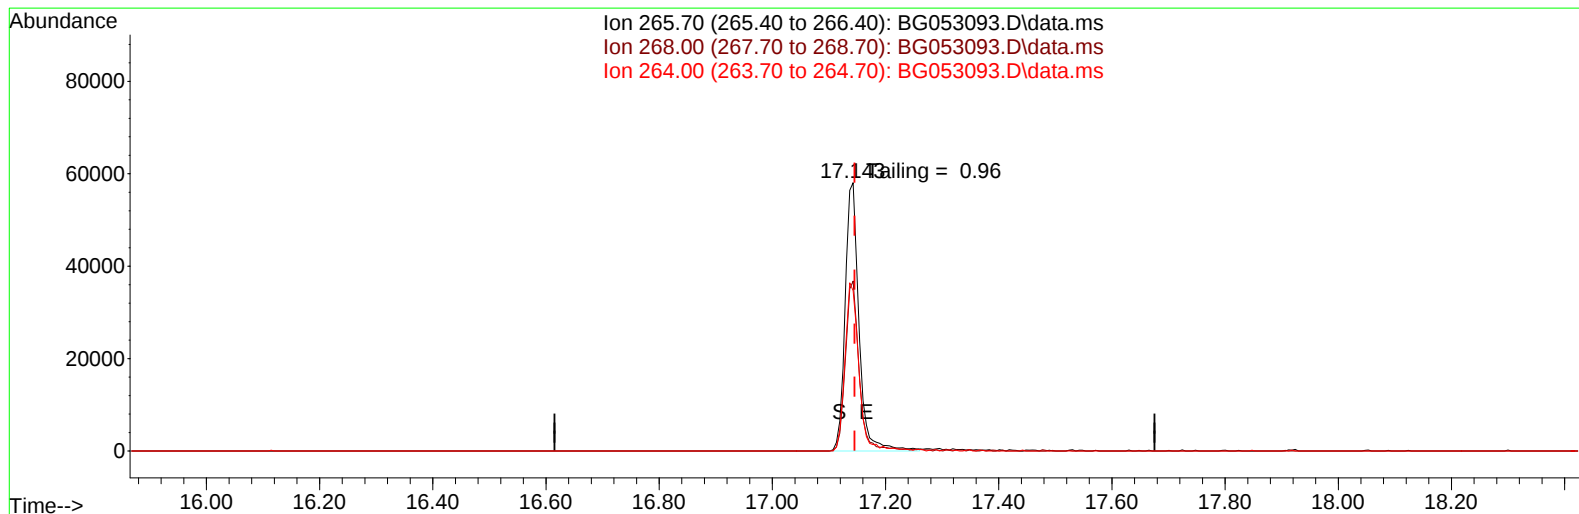

TIC: BG053093.D\data.ms

(70) Pentachlorophenol (C)




17.142min (-0.002) 24436.91 ng

response 98593

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	63.31
264.00	56.60	59.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041122\
 Data File : BG053093.D
 Acq On : 11 Apr 2022 9:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 08:19:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 15:31:24 2022
 Response via : Initial Calibration

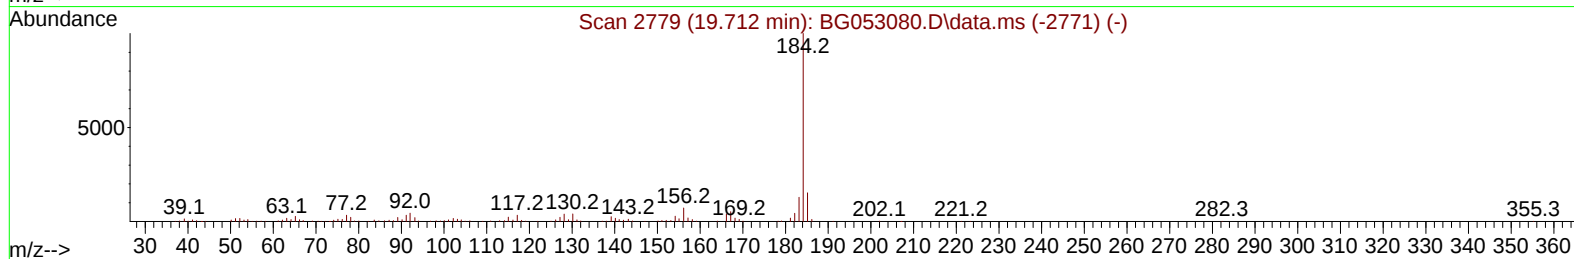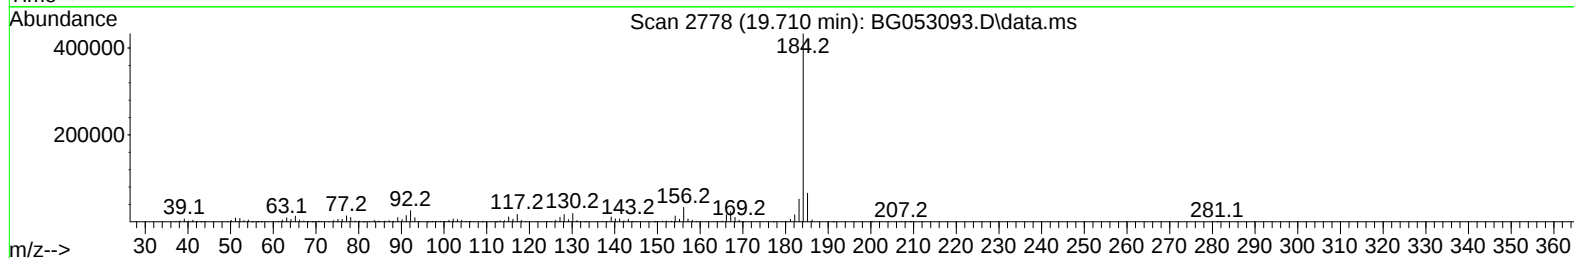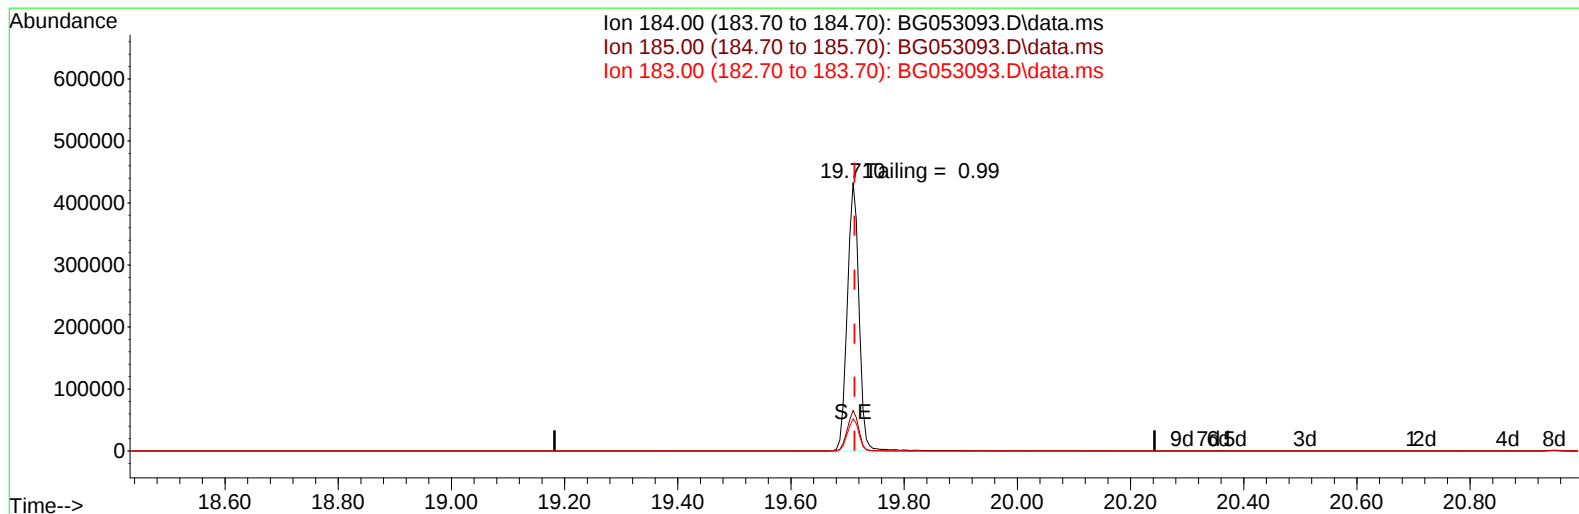

TIC: BG053093.D\data.ms

(77) Benzidine

19.710min (-0.002) 357601.82 ng m

response 622380

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.15
183.00	11.80	12.04
0.00	0.00	0.00