


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041122\
Data File : BG053093.D
Acq On : 11 Apr 2022 9:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 08 15:31:24 2022

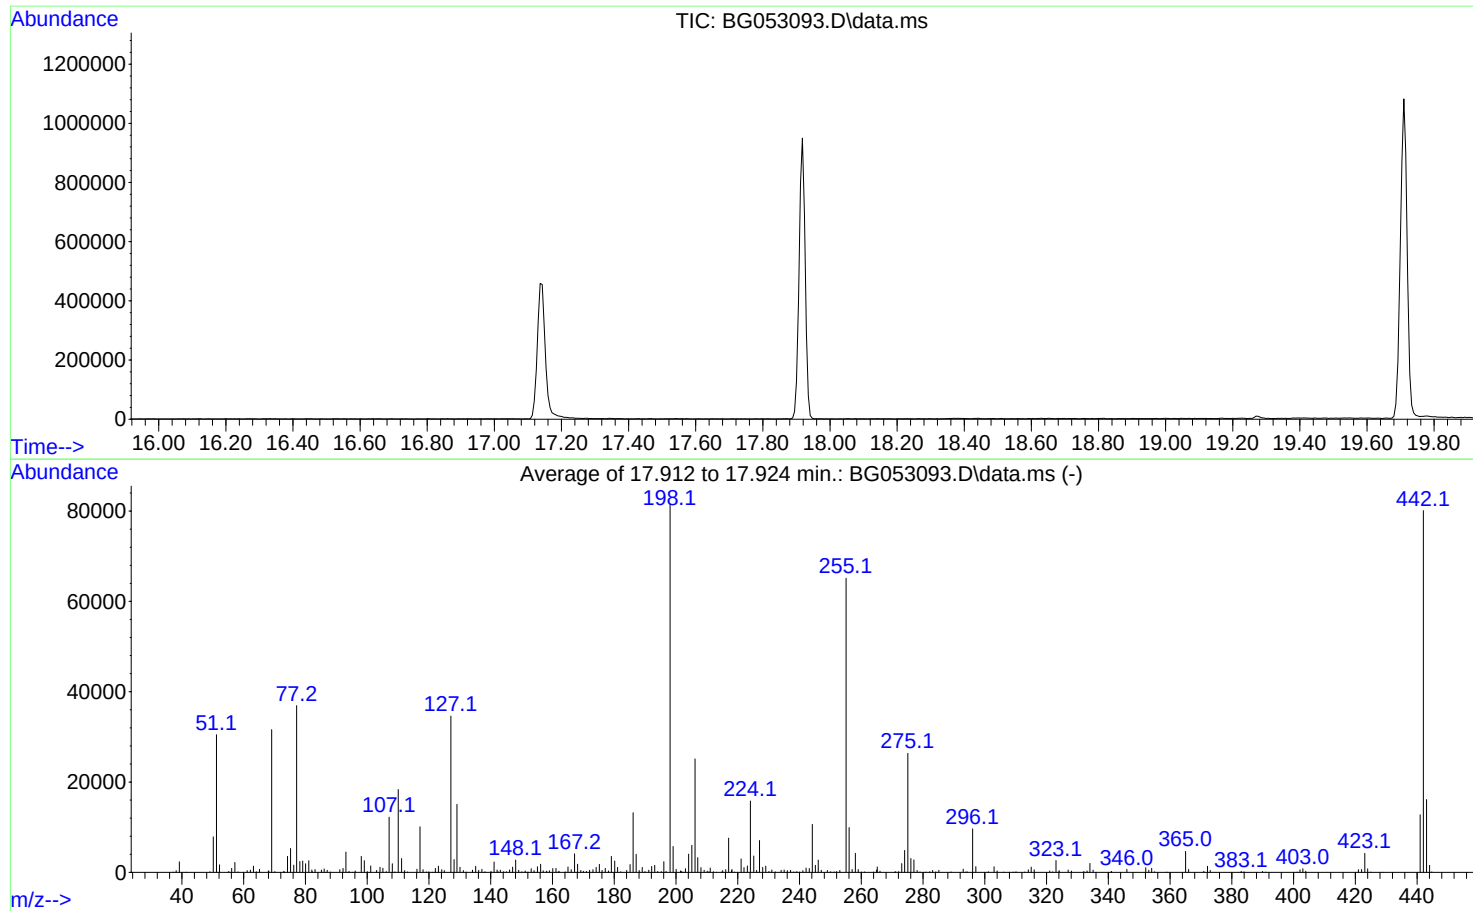




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	30475	PASS
68	69	0.00	2	1.2	375	PASS
69	198	0.00	100	38.8	31600	PASS
70	69	0.00	2	0.6	189	PASS
127	198	10	80	42.5	34619	PASS
197	198	0.00	2	0.3	228	PASS
198	198	100	100	100.0	81451	PASS
199	198	5	9	7.1	5750	PASS
275	198	10	60	32.4	26363	PASS
365	198	1	100	5.7	4658	PASS
441	198	0.01	100	15.7	12766	PASS
442	442	50	100	100.0	80123	PASS
443	442	15	24	20.1	16130	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041122\
Data File : BG053093.D
Acq On : 11 Apr 2022 9:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 12 08:19:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

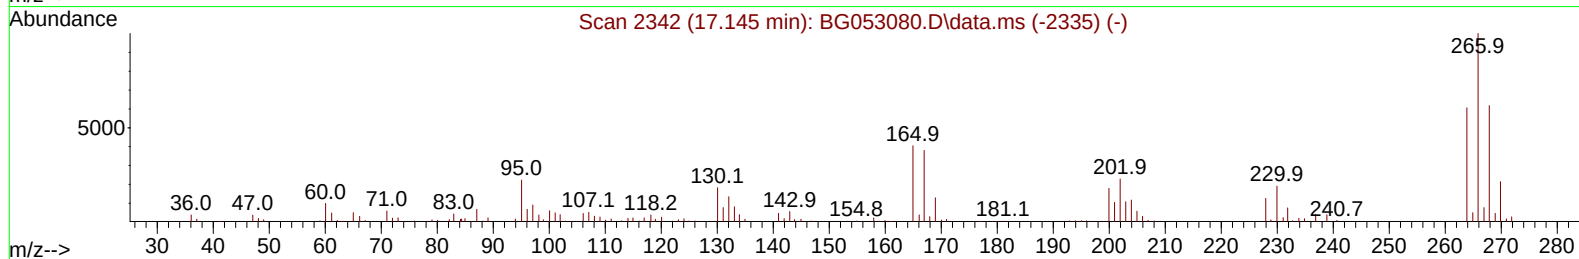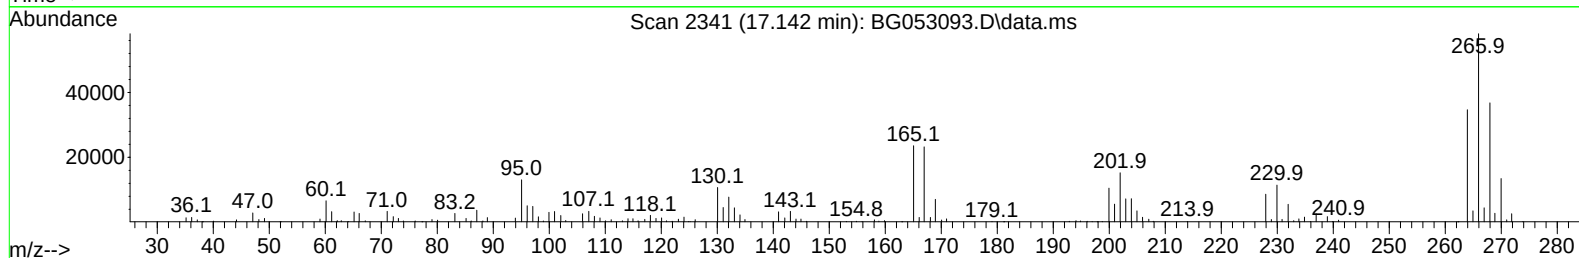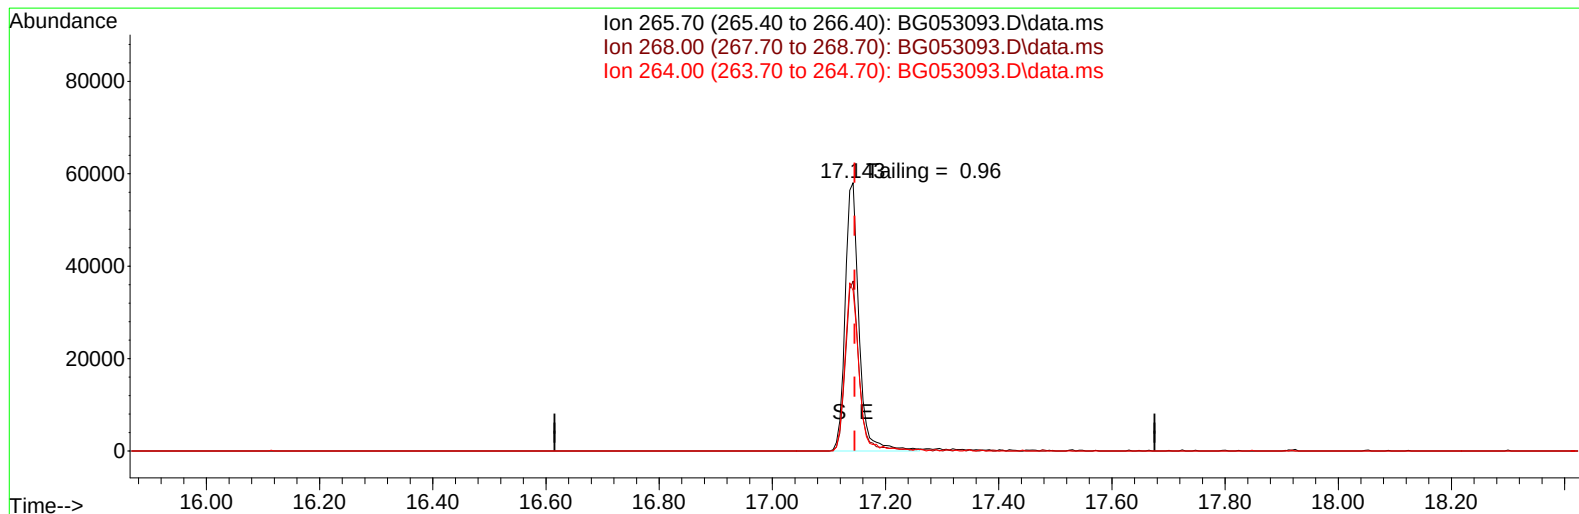

TIC: BG053093.D\data.ms

(70) Pentachlorophenol (C)

17.142min (-0.002) 24436.91 ng




response 98593

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	63.31
264.00	56.60	59.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041122\
 Data File : BG053093.D
 Acq On : 11 Apr 2022 9:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 12 08:19:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 15:31:24 2022
 Response via : Initial Calibration

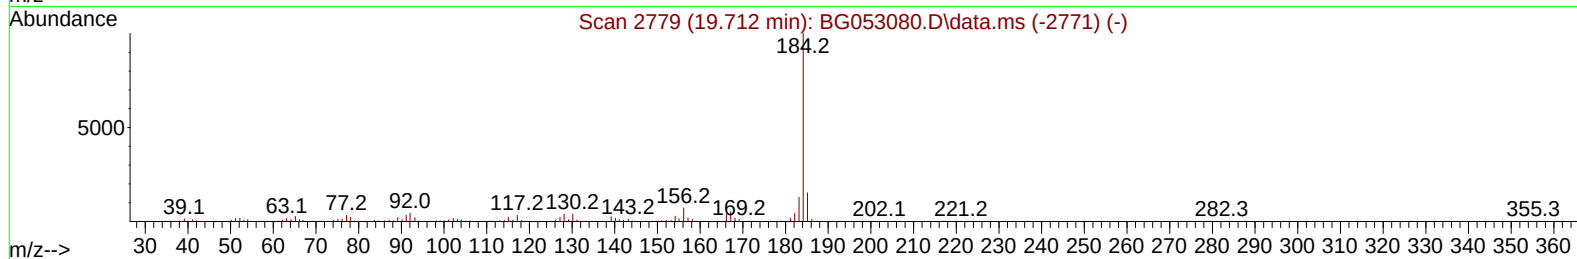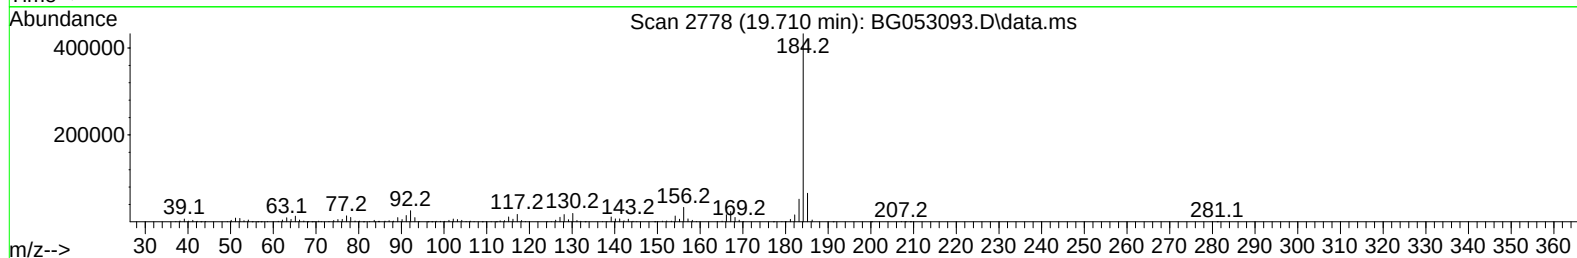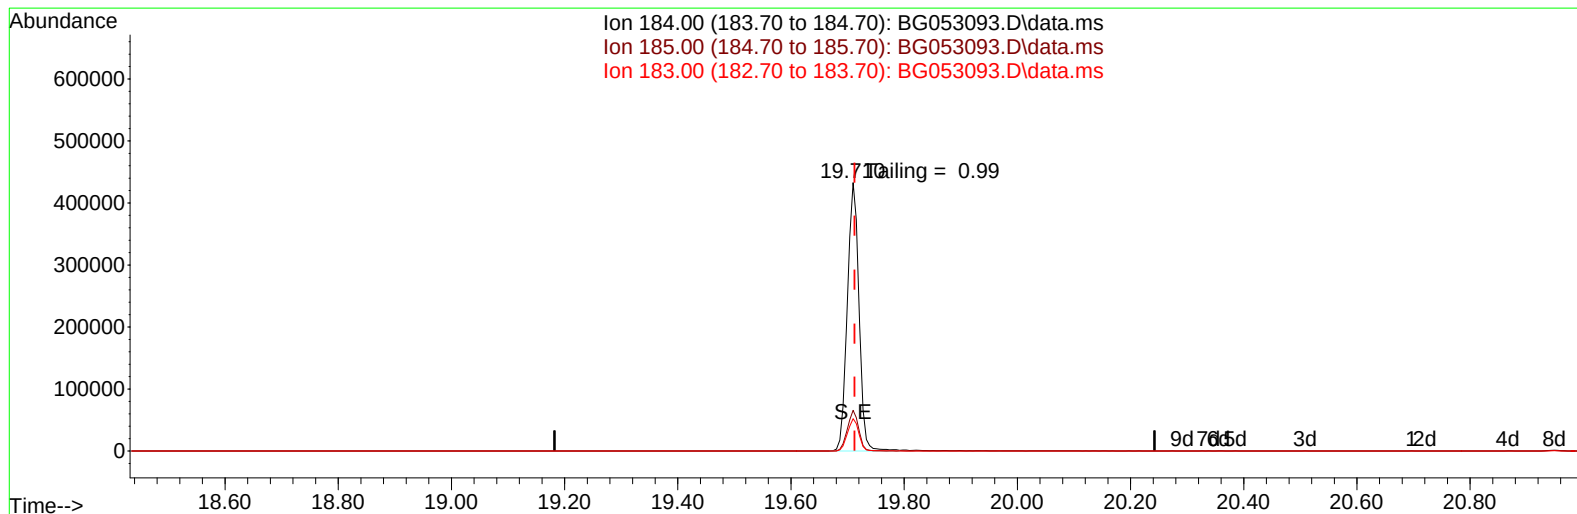

TIC: BG053093.D\data.ms

(77) Benzidine

19.710min (-0.002) 357601.82 ng m

response 622380

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.15
183.00	11.80	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/11/2022	BNA_G	<u>BG053093.D</u>
Compound Name	Response	Retention Time
DDT	331306	20.949
DDD	4817	20.503
DDE	970	19.997
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5787	337093	1.72

Instrument :
BNA_G
ClientSampleId :
DFTPP