
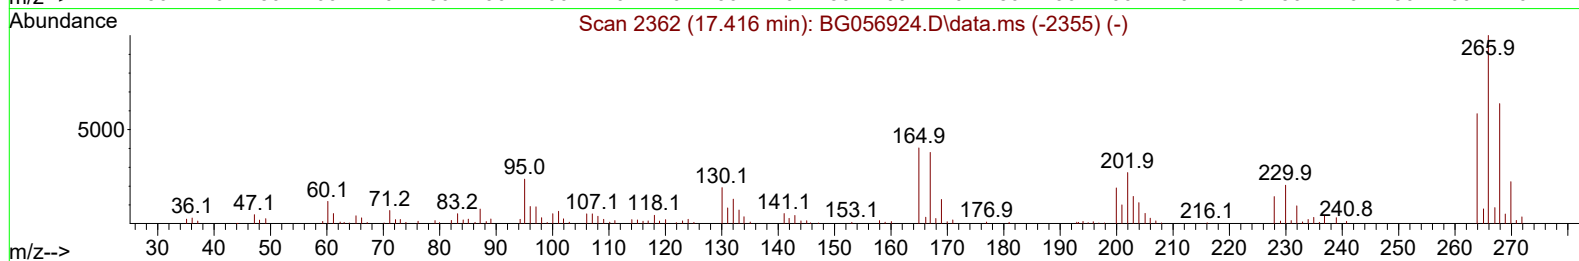
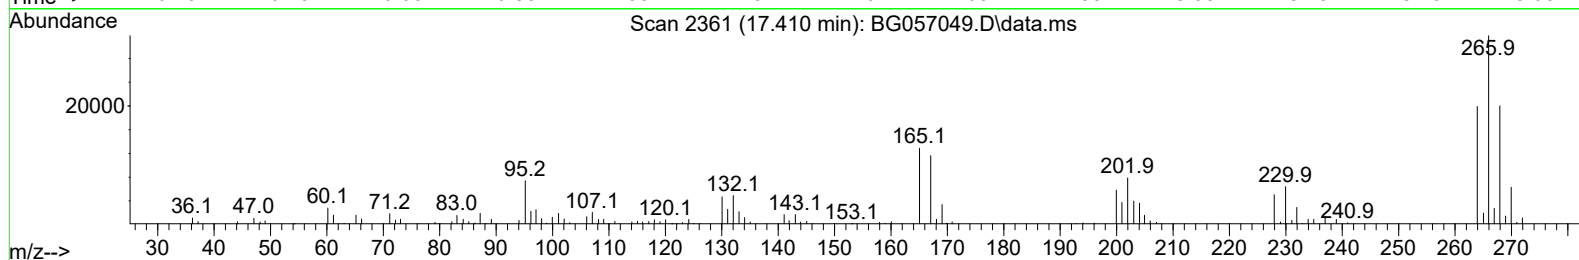


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041123\
Data File : BG057049.D
Acq On : 11 Apr 2023 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 05:07:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 04:45:47 2023
Response via : Initial Calibration

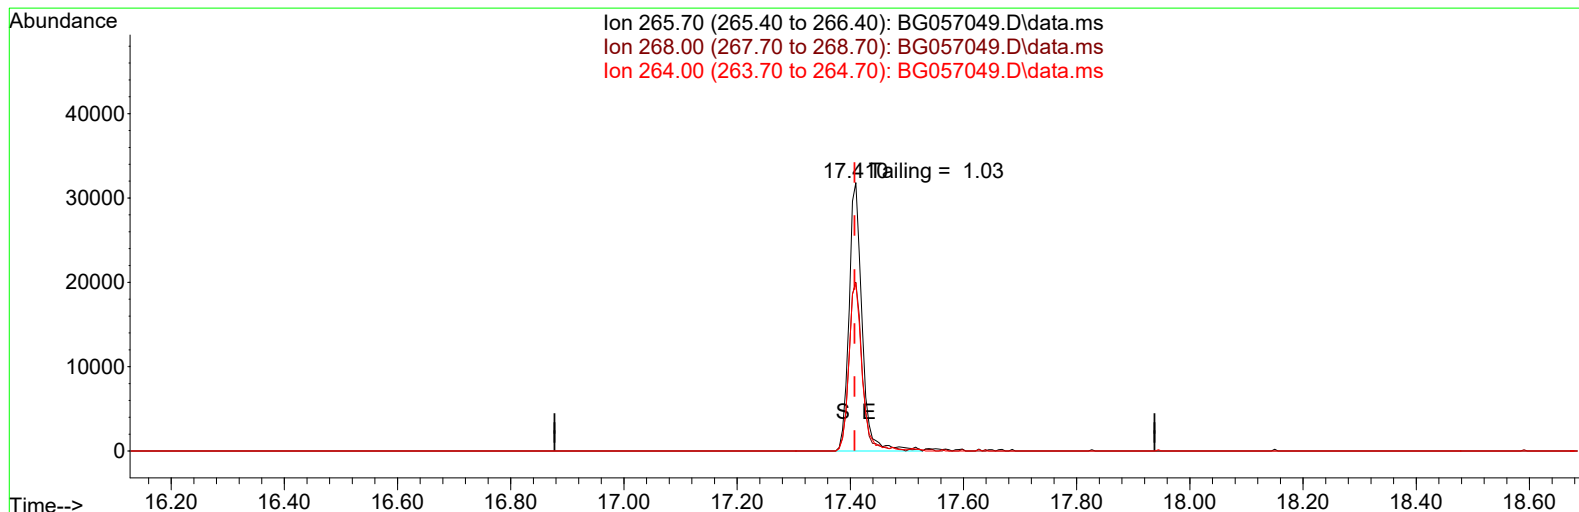

TIC: BG057049.D\data.ms

(70) Pentachlorophenol (C)




17.410min (+ 0.002) 102293.94 ng

response 50273

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.87
264.00	58.50	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041123\
Data File : BG057049.D
Acq On : 11 Apr 2023 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 05:07:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 04:45:47 2023
Response via : Initial Calibration

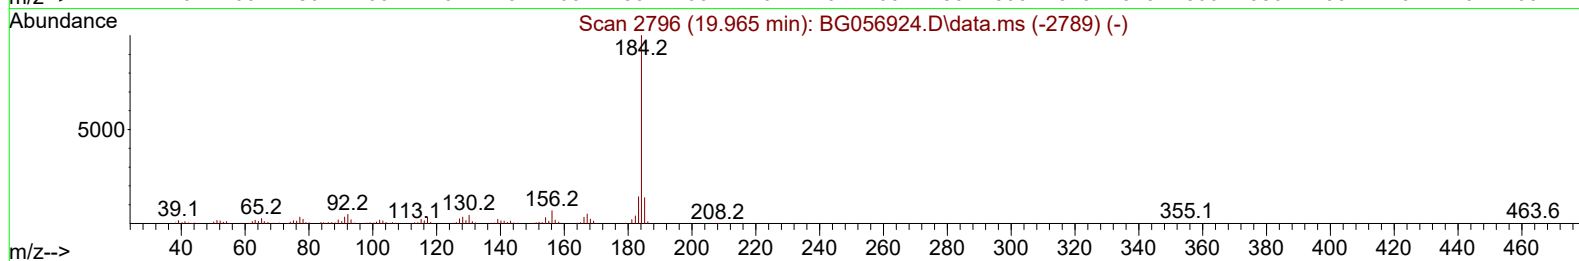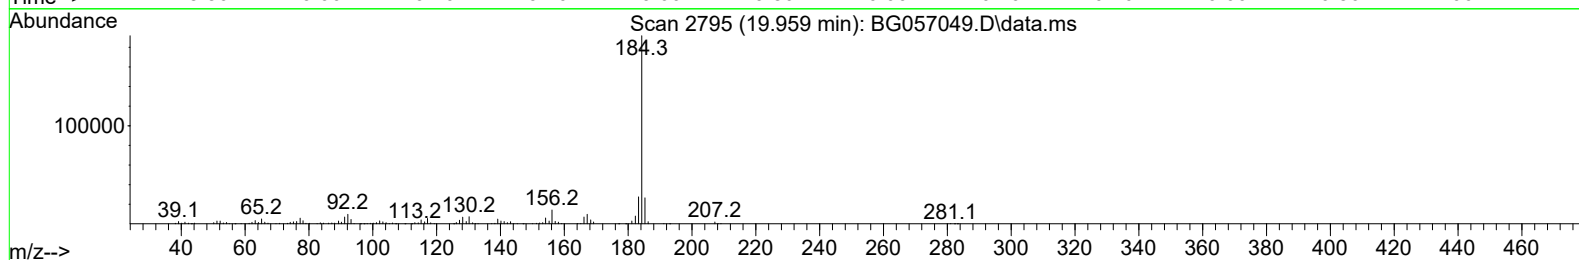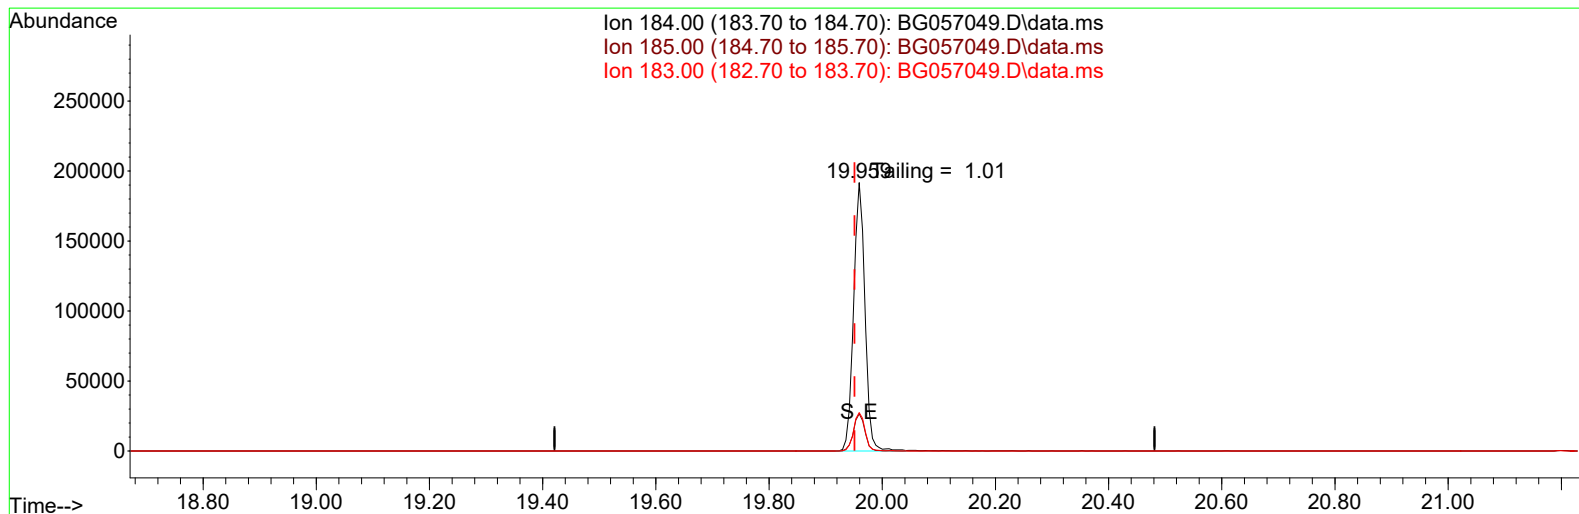

TIC: BG057049.D\data.ms

(77) Benzidine**19.959min (+ 0.008) 8539.51 ng****response 268191**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.87
183.00	14.20	14.34
0.00	0.00	0.00