


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041123\
Data File : BG057049.D
Acq On : 11 Apr 2023 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Apr 08 04:45:47 2023

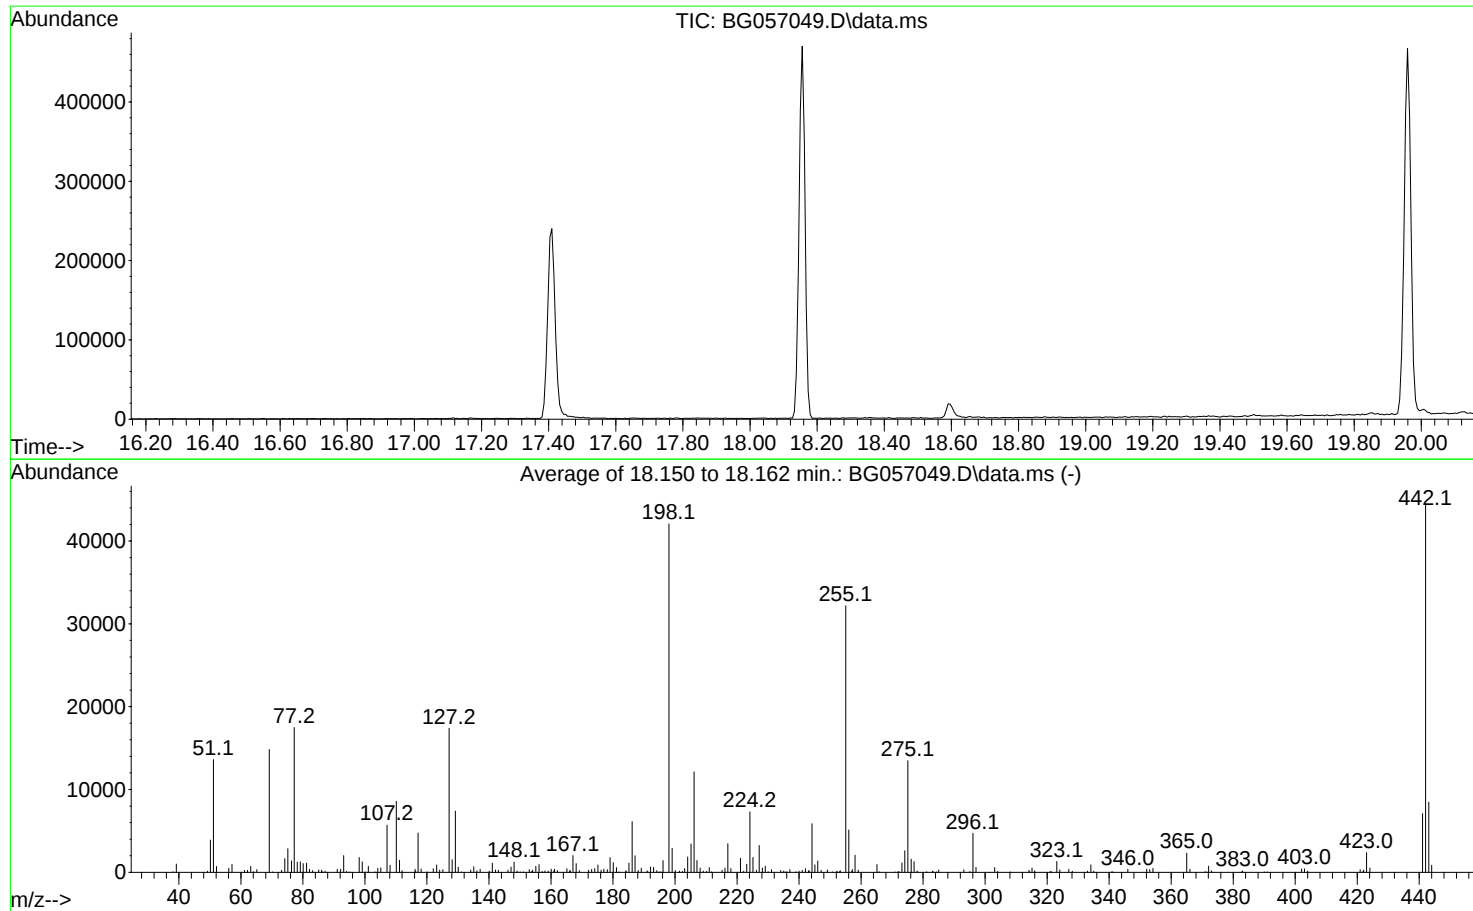




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	13606	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.2	14827	PASS
70	69	0.00	2	0.4	54	PASS
127	198	10	80	41.3	17380	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42085	PASS
199	198	5	9	6.9	2897	PASS
275	198	10	60	32.0	13481	PASS
365	198	1	100	5.5	2304	PASS
441	198	0.01	100	16.8	7074	PASS
442	442	50	100	100.0	44424	PASS
443	442	15	24	19.1	8480	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041123\
Data File : BG057049.D
Acq On : 11 Apr 2023 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 12 05:07:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 04:45:47 2023
Response via : Initial Calibration

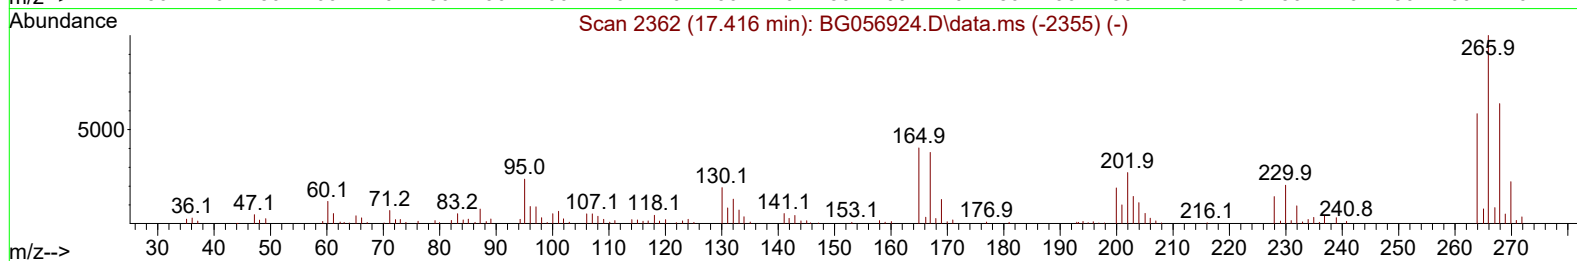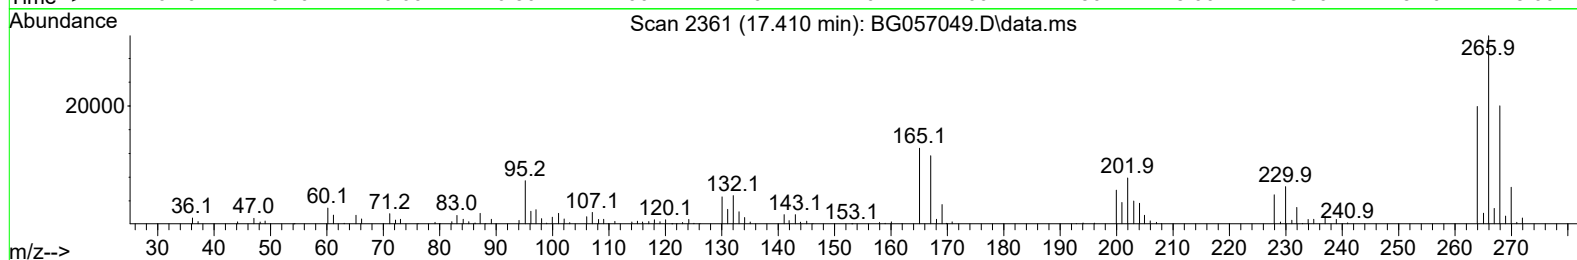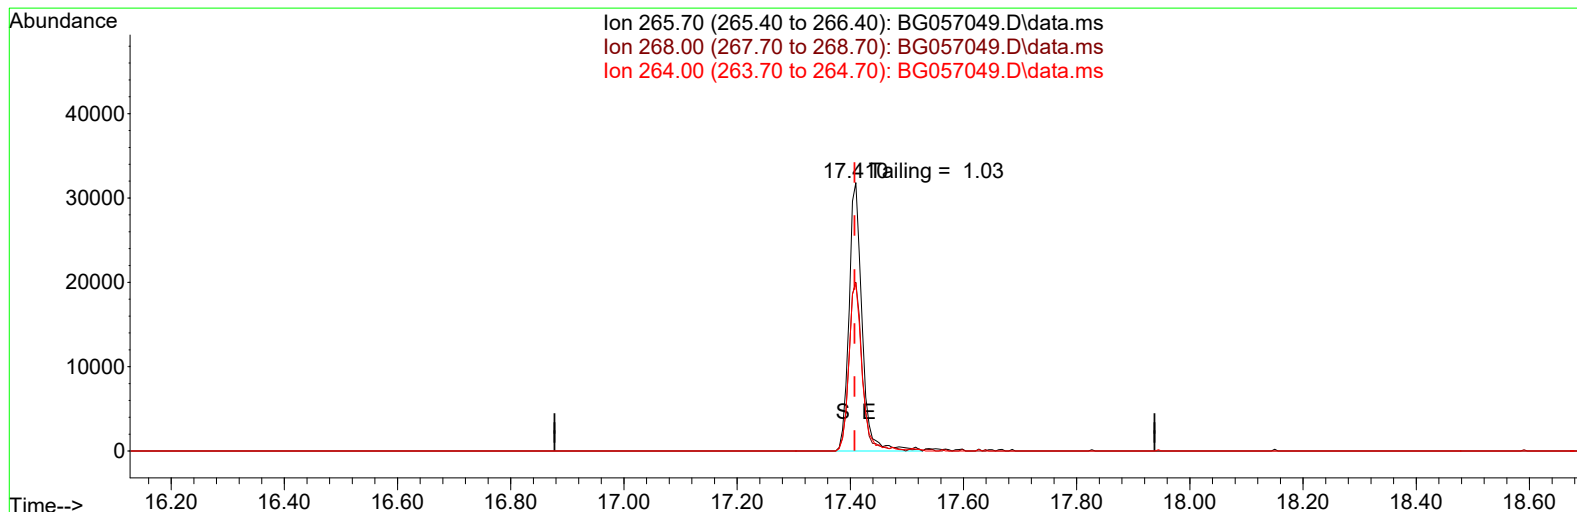

TIC: BG057049.D\data.ms

(70) Pentachlorophenol (C)

17.410min (+ 0.002) 102293.94 ng




response 50273

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.87
264.00	58.50	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041123\
Data File : BG057049.D
Acq On : 11 Apr 2023 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 12 05:07:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 04:45:47 2023
Response via : Initial Calibration

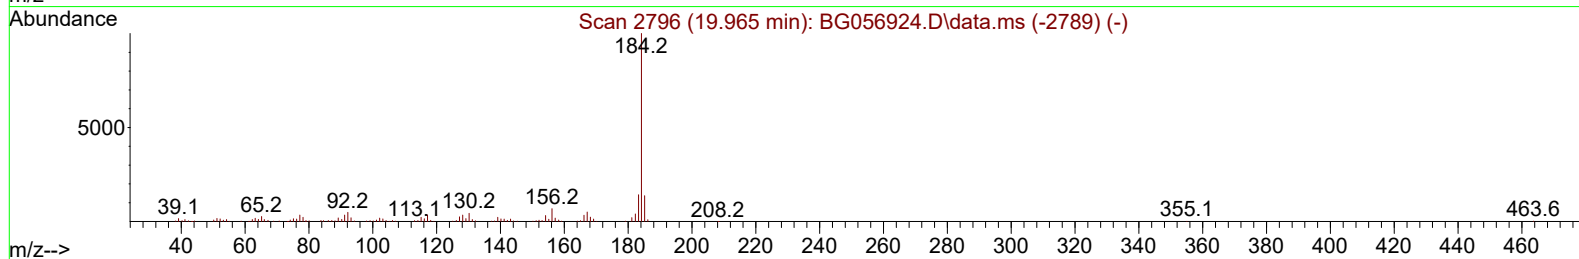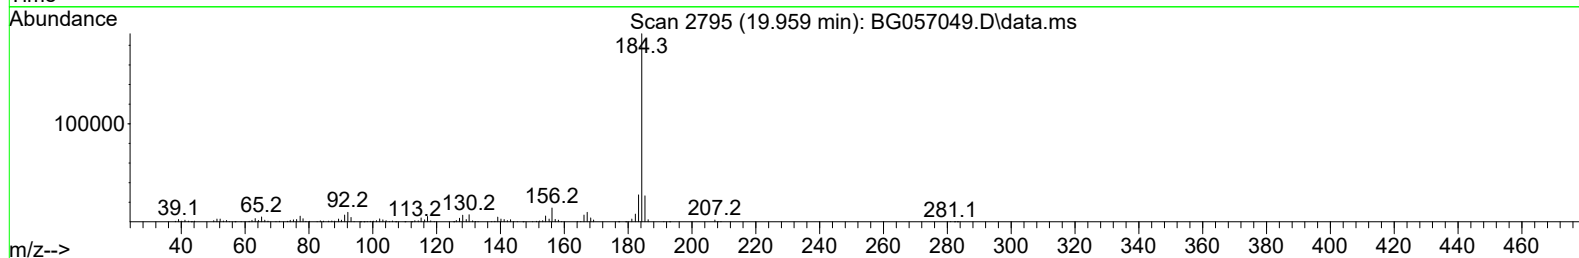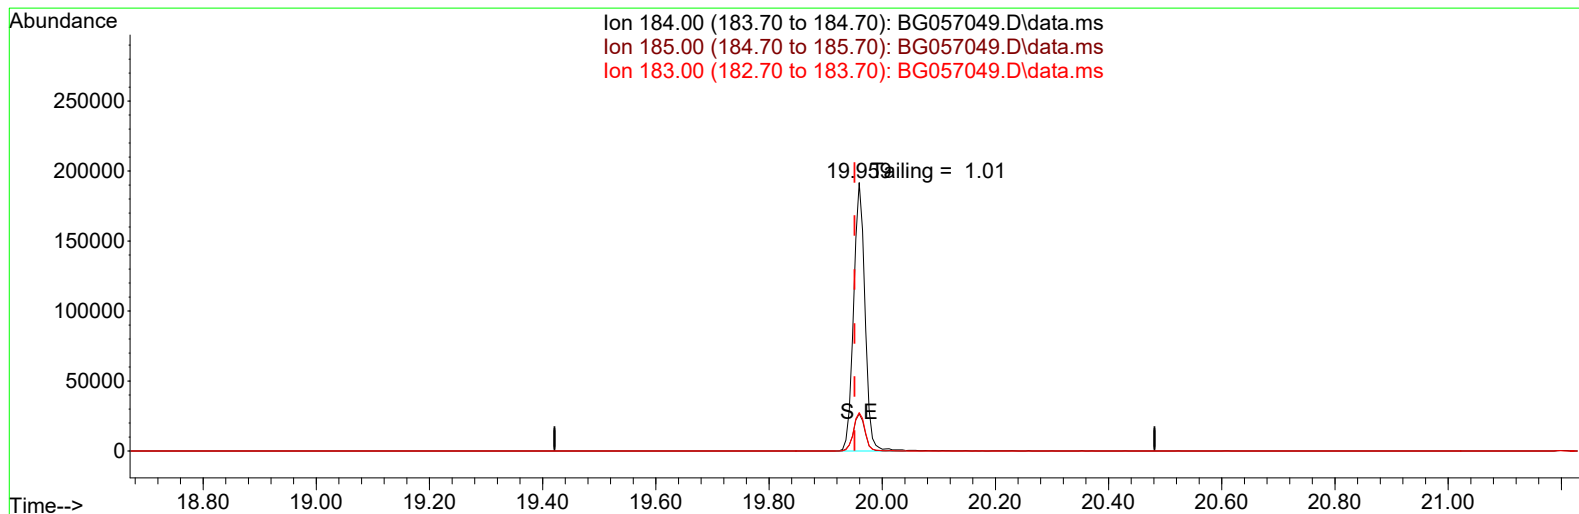

TIC: BG057049.D\data.ms

(77) Benzidine

19.959min (+ 0.008) 8539.51 ng

response 268191

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.87
183.00	14.20	14.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/11/2023	BNA_G	<u>BG057049.D</u>
Compound Name	Response	Retention Time
DDT	133115	21.205
DDD	3352	20.74
DDE	136	20.241
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3488	136603	2.55

Instrument :
BNA_G
ClientSampleId :
DFTPP