
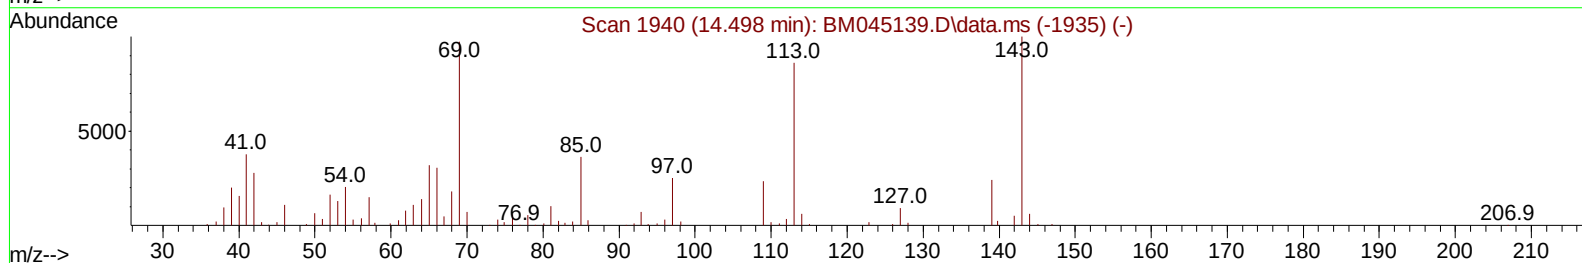
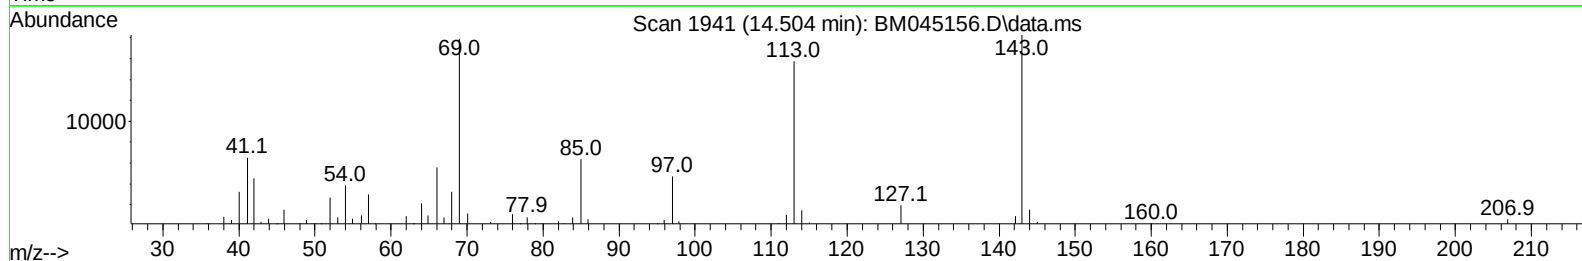


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045156.D
Acq On : 12 Apr 2024 05:02
Operator : MA/JU
Sample : PB160162BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 12 05:58:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

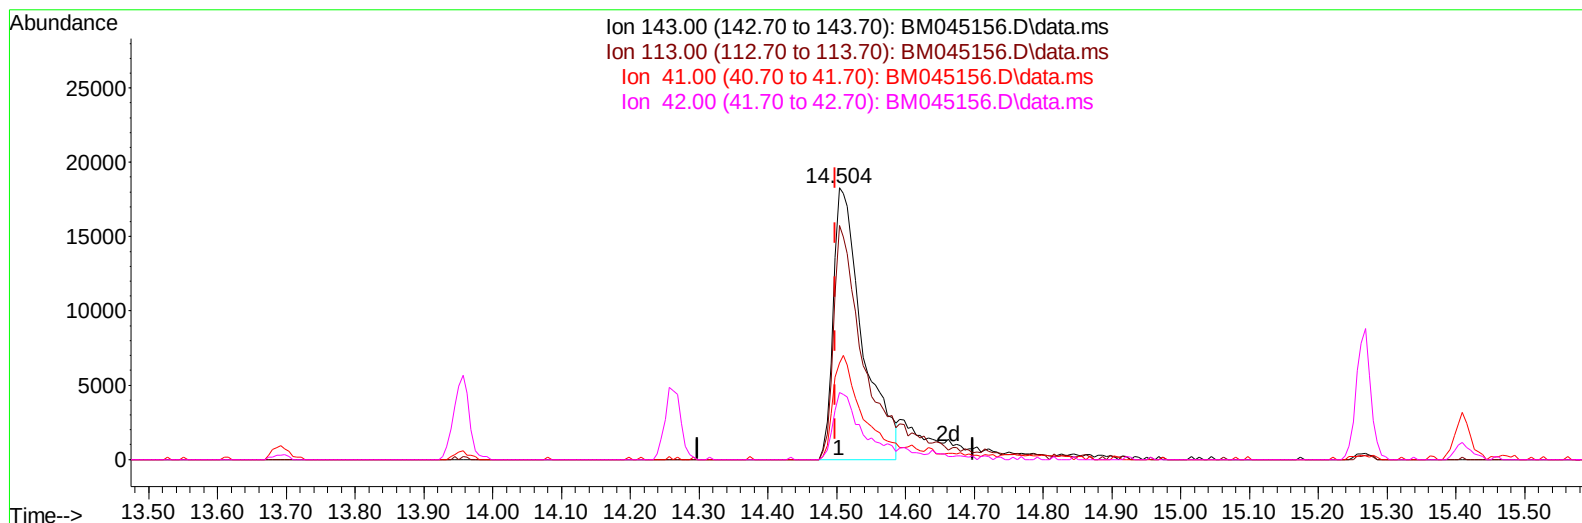

TIC: BM045156.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.504min (+ 0.006) 21.27 ng/ul

response 53601

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	86.14
41.00	36.50	35.44
42.00	23.30	24.78

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041124\
Data File : BM045156.D
Acq On : 12 Apr 2024 05:02
Operator : MA/JU
Sample : PB160162BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 12 05:58:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 11 18:54:49 2024
Response via : Initial Calibration

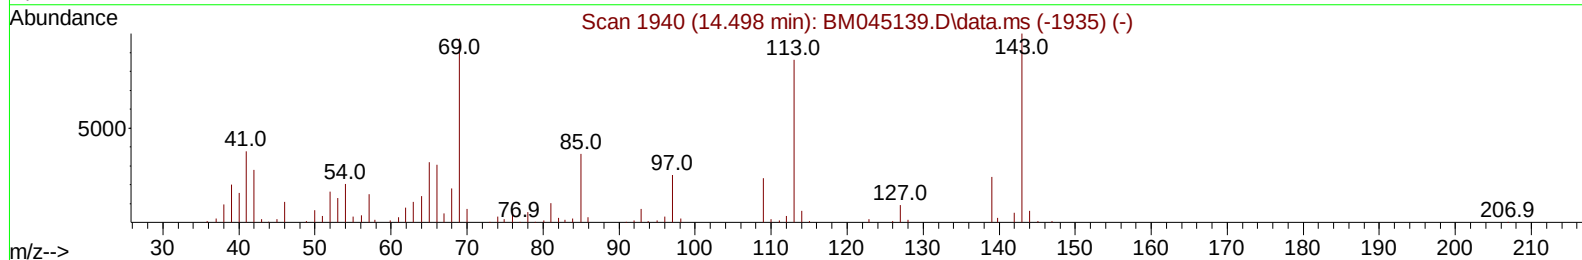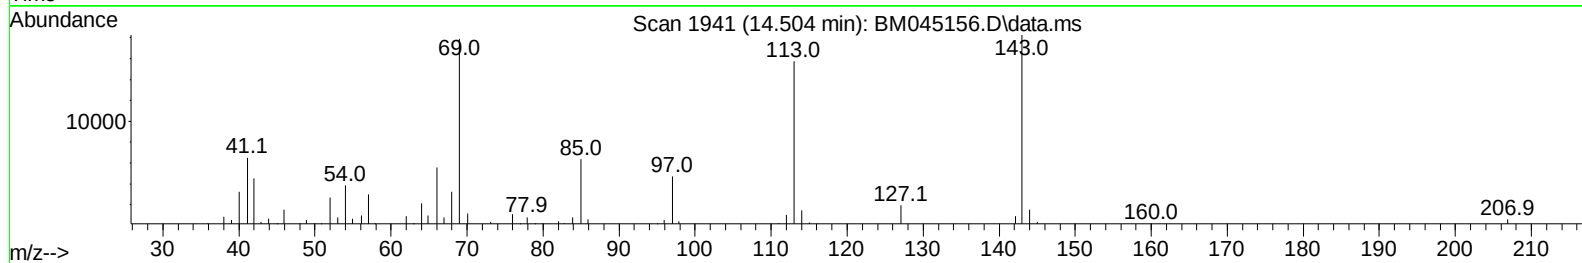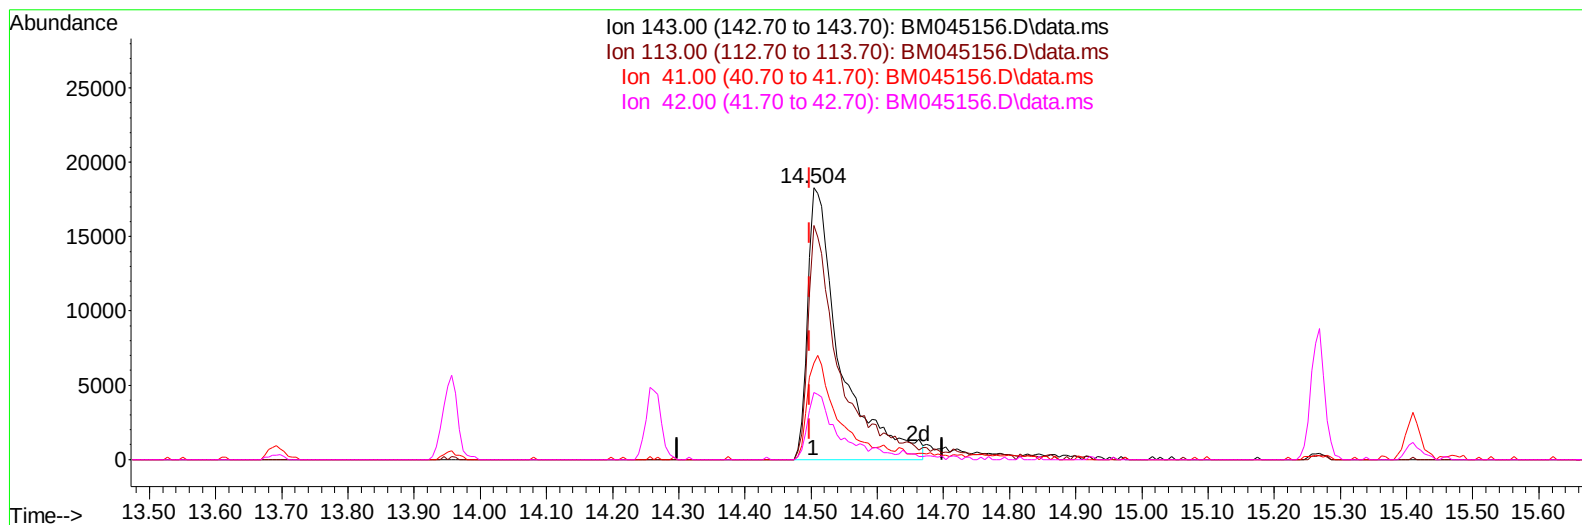

TIC: BM045156.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.504min (+ 0.006) 24.47 ng/ul m

response 61663

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	86.14
41.00	36.50	35.44
42.00	23.30	24.78

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041124\
Data File : BG060856.D
Acq On : 11 Apr 2024 11:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 06:08:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

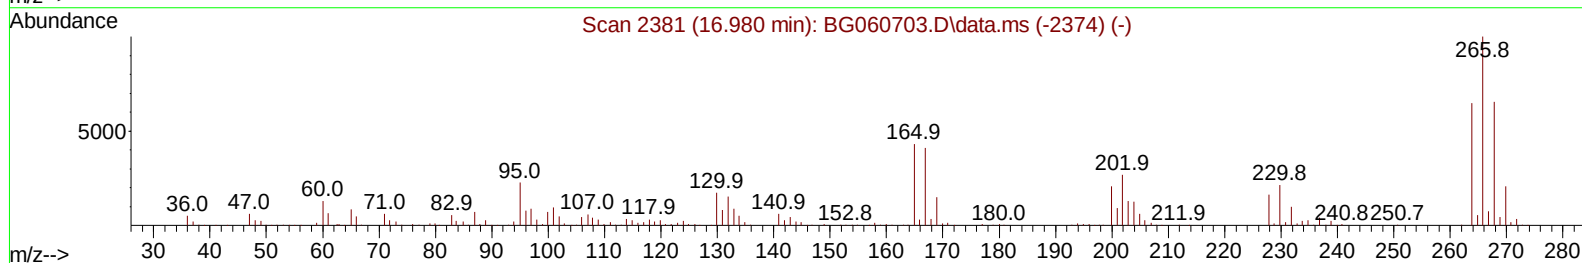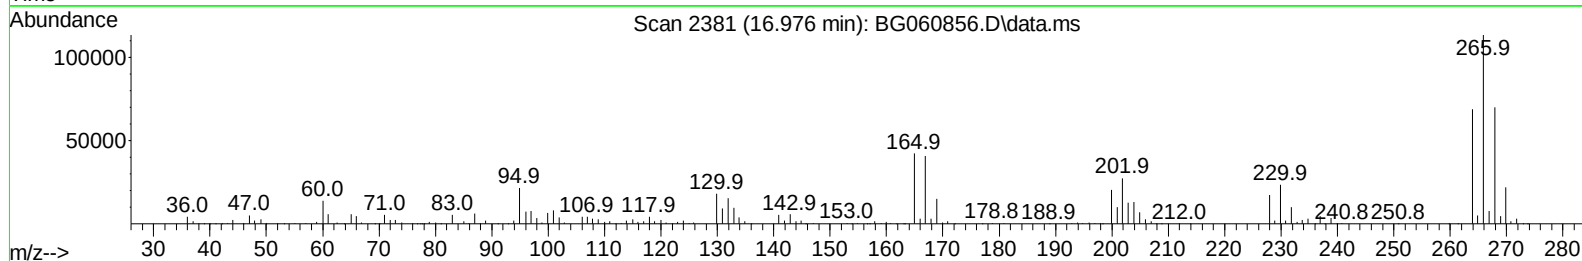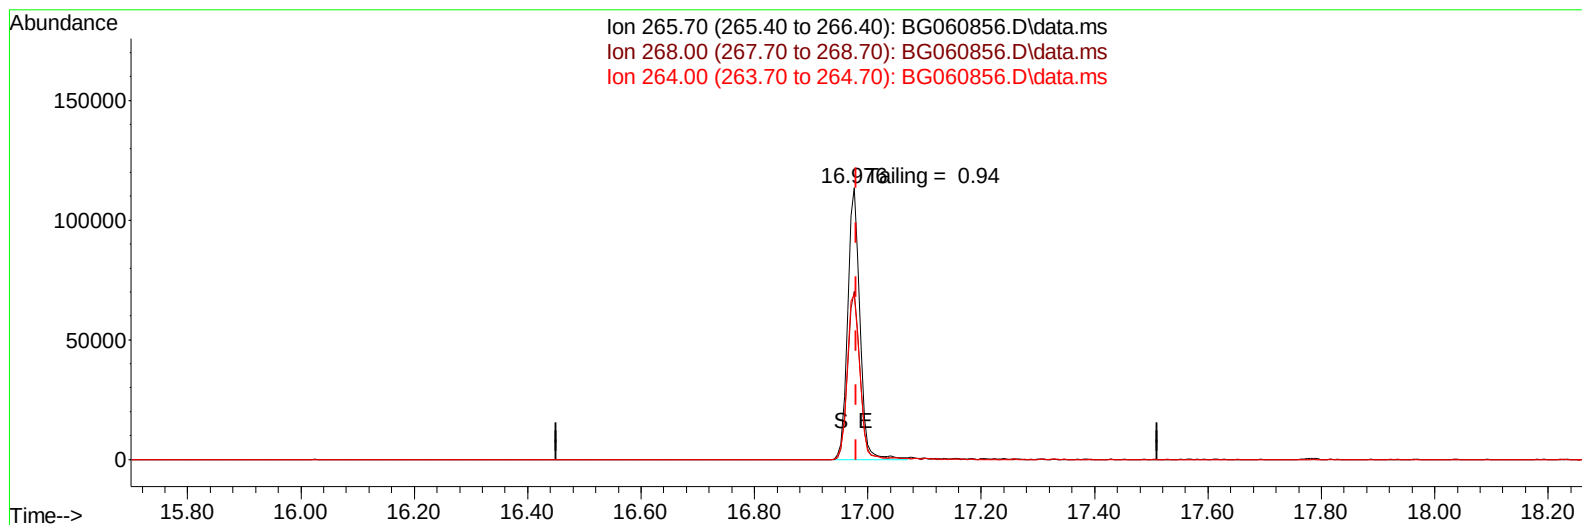




TIC: BG060856.D\data.ms

(70) Pentachlorophenol (C)**16.976min (-0.004) 303251.66 ng****response 170020**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	61.89
264.00	64.70	60.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041124\
Data File : BG060856.D
Acq On : 11 Apr 2024 11:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 06:08:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

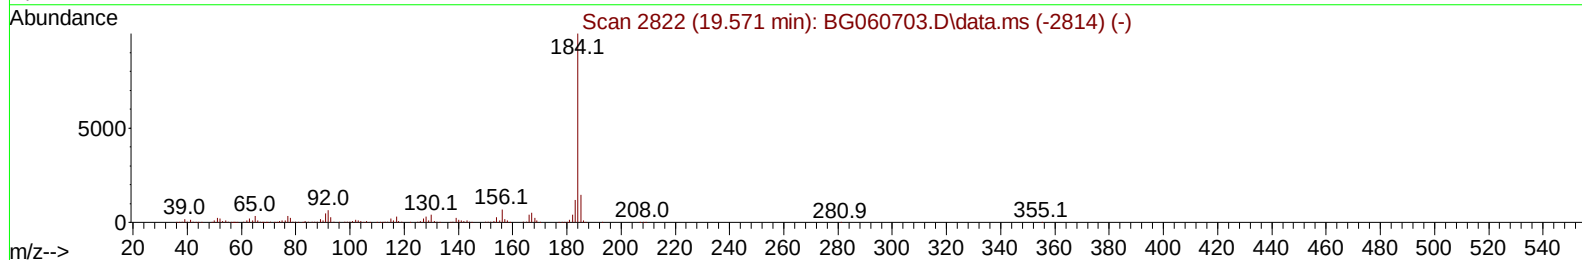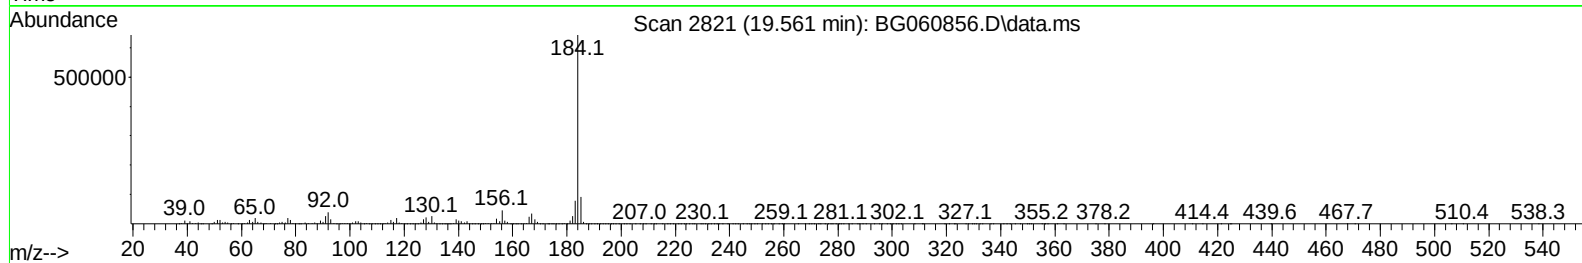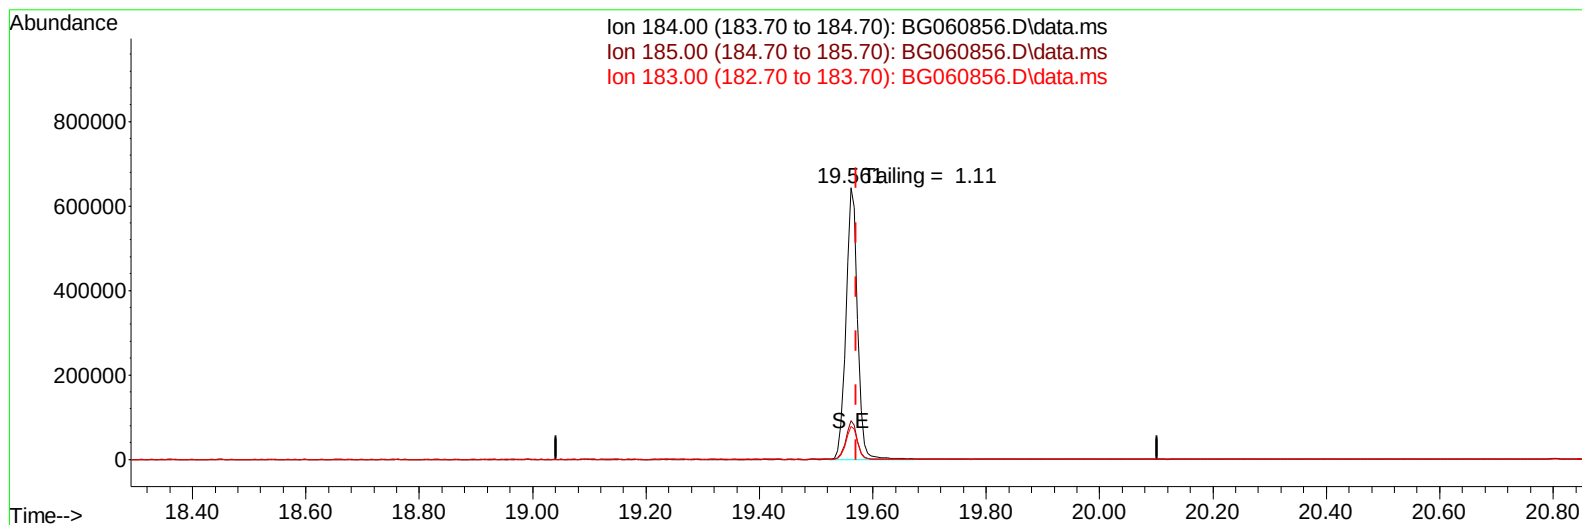

TIC: BG060856.D\data.ms

(77) Benzidine**19.561min (-0.010) 129045.82 ng****response 920873**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.32
183.00	11.90	12.16
0.00	0.00	0.00