
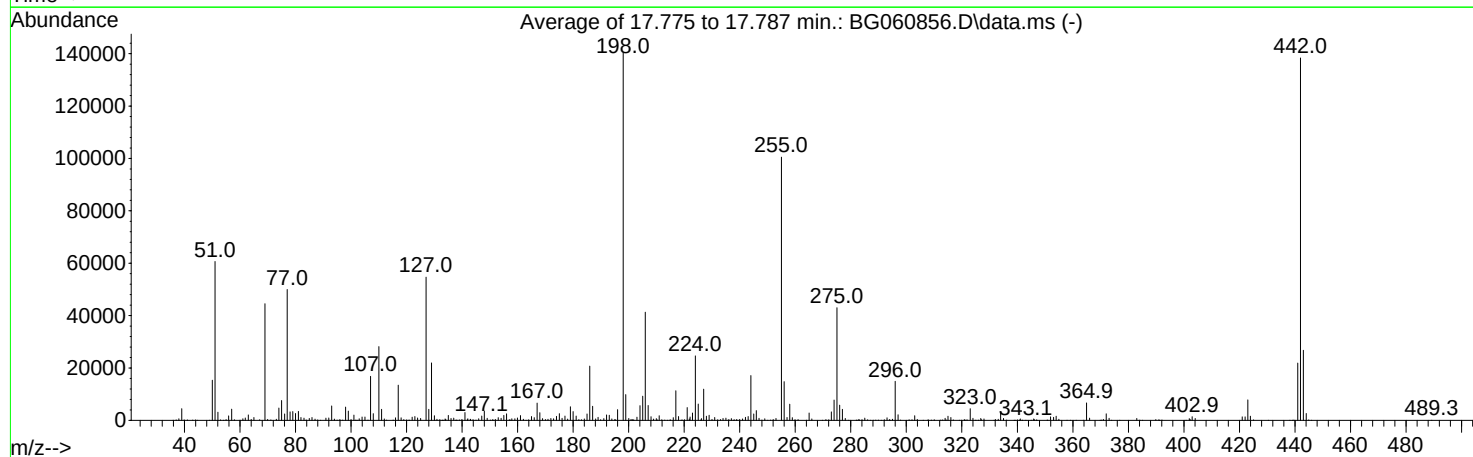


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041124\
Data File : BG060856.D
Acq On : 11 Apr 2024 11:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

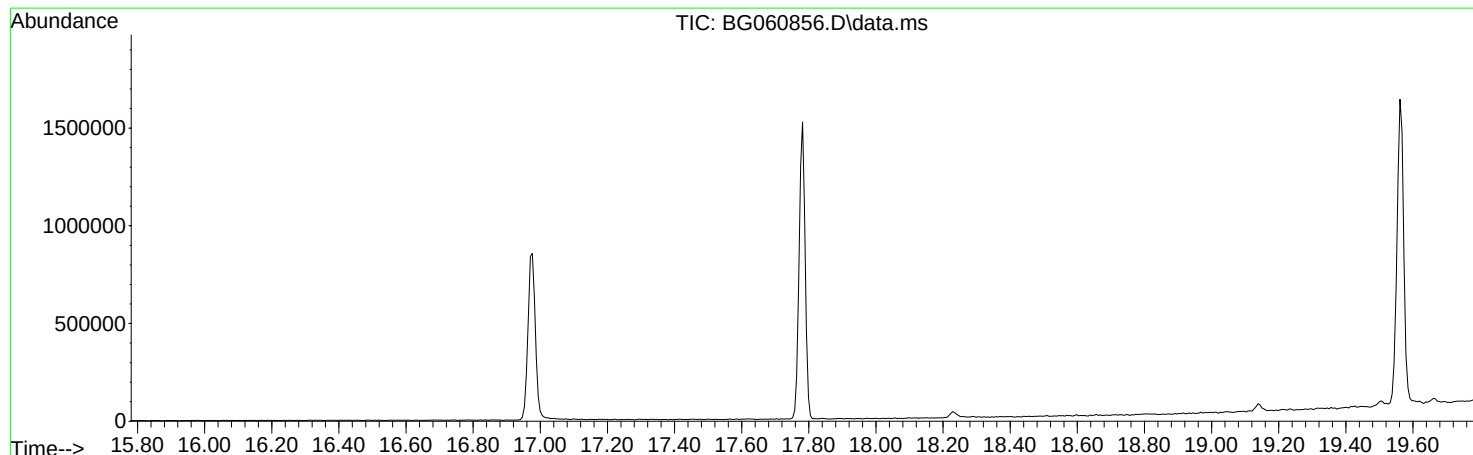

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	60691	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.7	44559	PASS
70	69	0.00	2	0.8	355	PASS
127	198	10	80	38.9	54699	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140445	PASS
199	198	5	9	7.0	9839	PASS
275	198	10	60	30.6	43027	PASS
365	198	1	100	4.8	6683	PASS
441	198	0.01	100	15.6	21891	PASS
442	442	50	100	100.0	138365	PASS
443	442	15	24	19.3	26749	PASS