
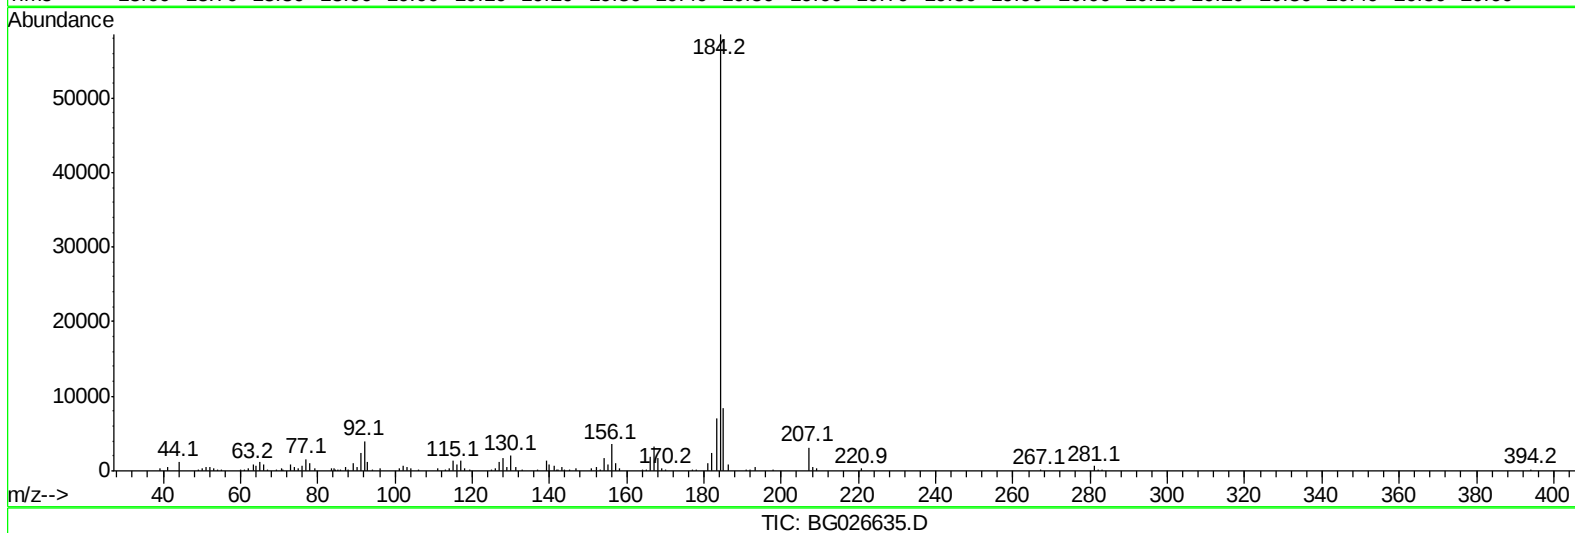


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041217\
Data File : BG026635.D
Acq On : 12 Apr 2017 12:54
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 03:47:37 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

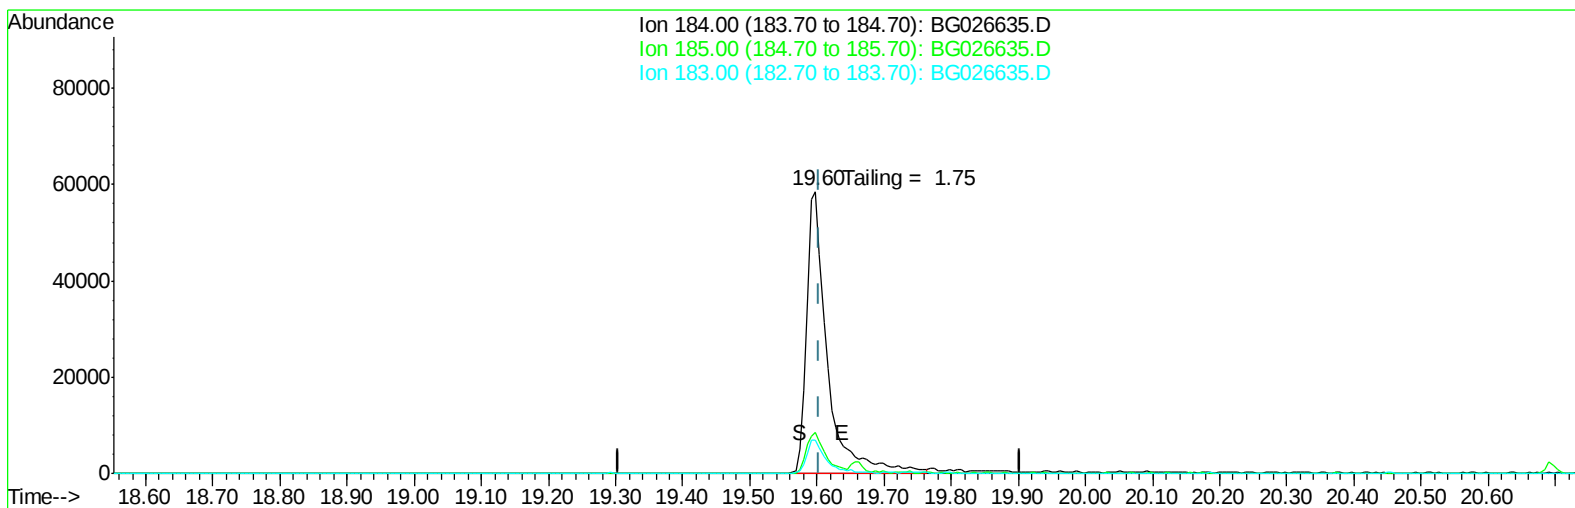

(76) Benzidine



19.598min (-0.006) 60142.80ng

response 122344

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.42
183.00	13.80	12.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041217\
Data File : BG026635.D
Acq On : 12 Apr 2017 12:54
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 03:47:37 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 17:43:27 2017
Response via : Initial Calibration

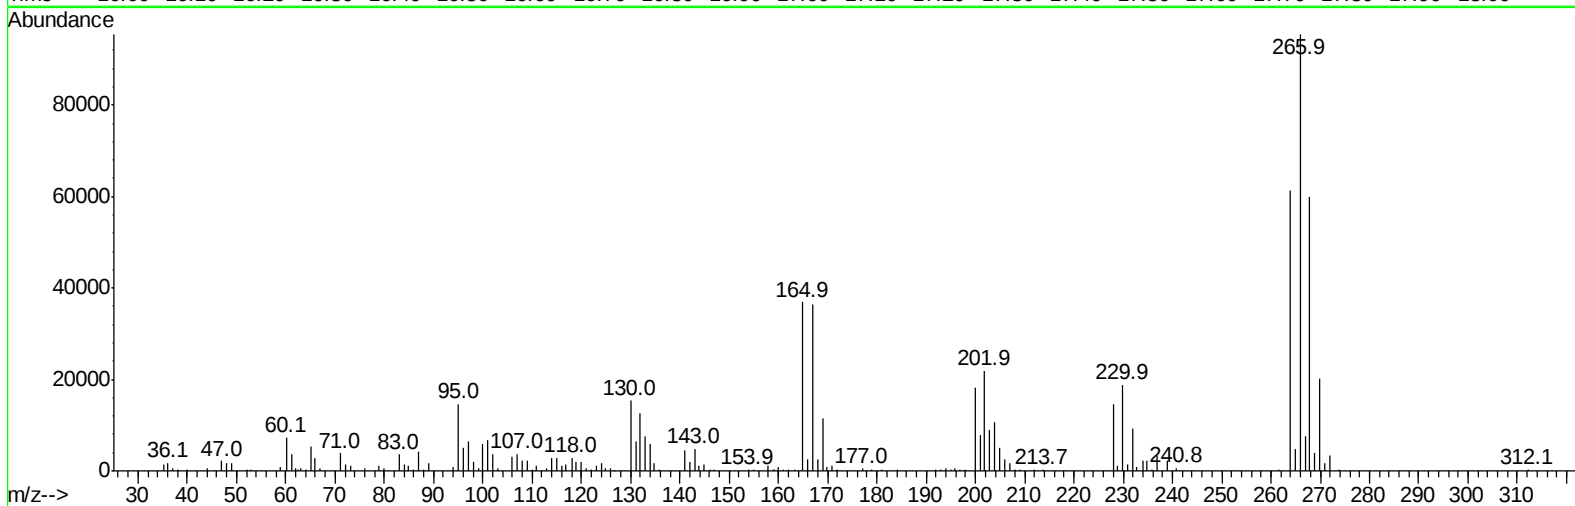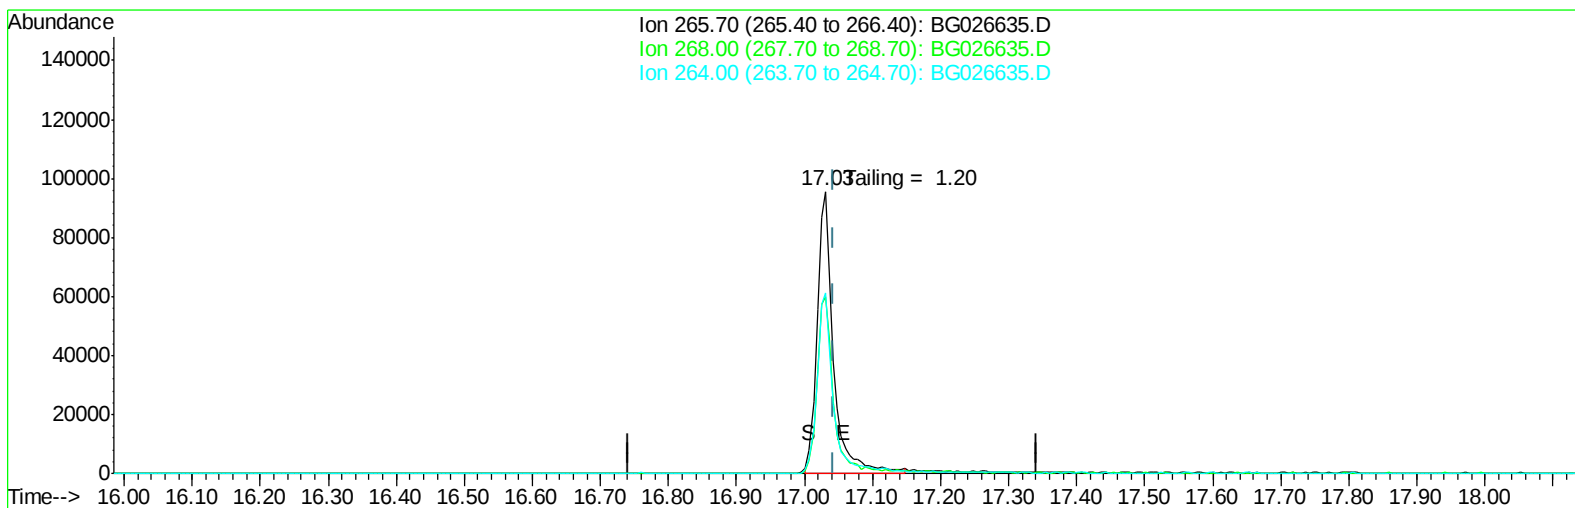

TIC: BG026635.D

(69) Pentachlorophenol (C)

17.031min (-0.012) 388797.01ng

response 160976

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.64
264.00	62.60	64.10
0.00	0.00	0.00