
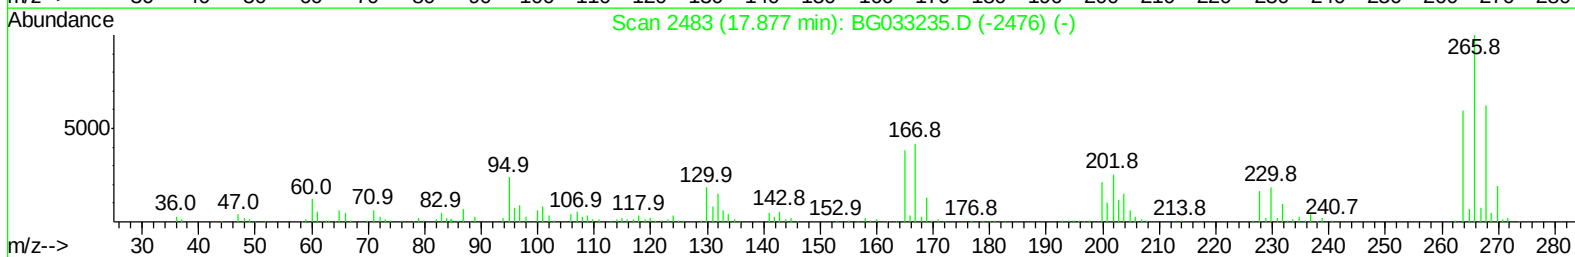
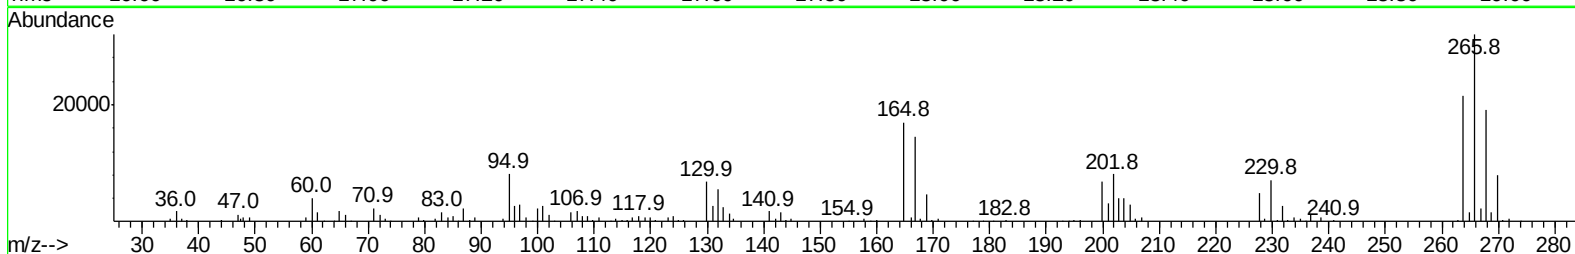


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041218\
Data File : BG033773.D
Acq On : 12 Apr 2018 15:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 04:45:46 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 16:51:36 2018
Response via : Initial Calibration

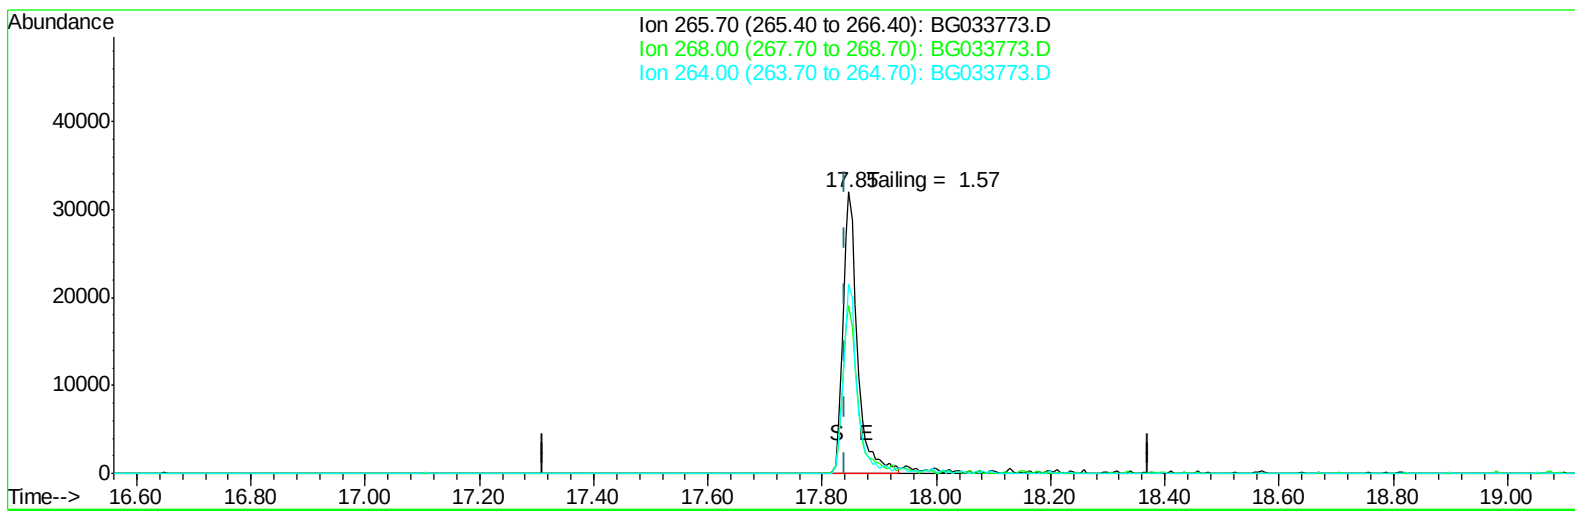

TIC: BG033773.D

(69) Pentachlorophenol (C)




17.846min (+0.006) 0.00ng

response 57197

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.60
264.00	62.00	67.33
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041218\
Data File : BG033773.D
Acq On : 12 Apr 2018 15:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 04:45:46 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 16:51:36 2018
Response via : Initial Calibration

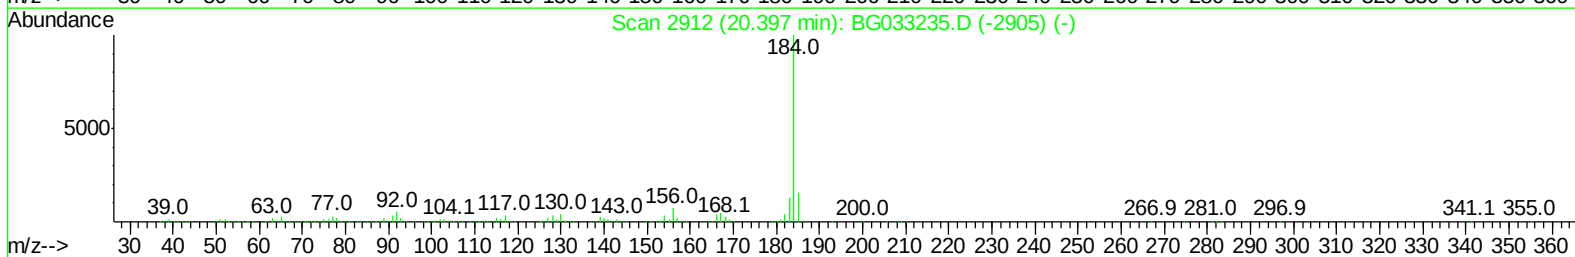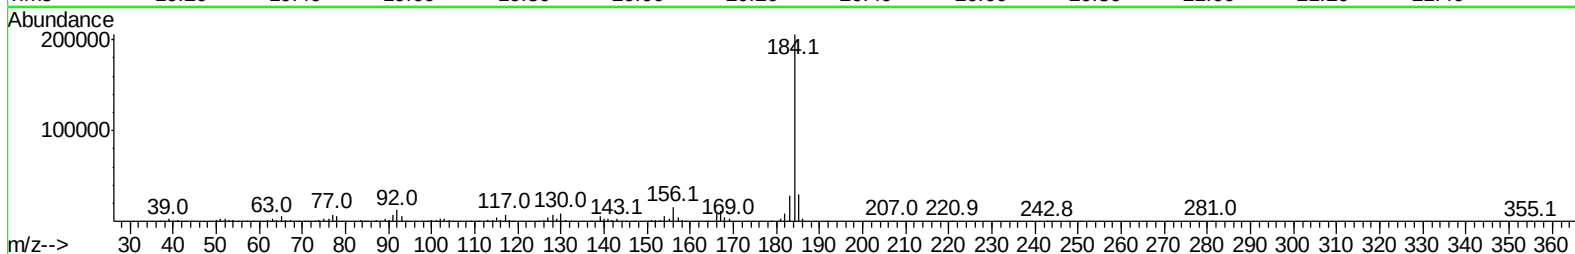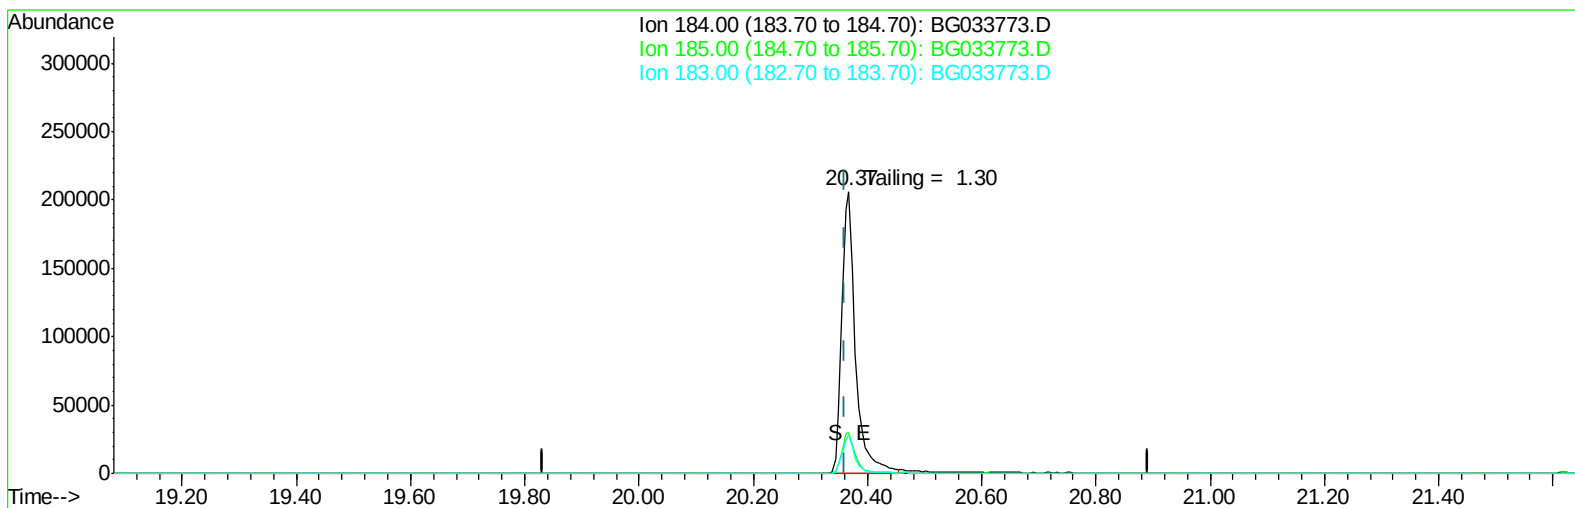

TIC: BG033773.D

(76) Benzidine

20.367min (+0.006) 192034.46ng

response 354123

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.43
183.00	13.30	13.63
0.00	0.00	0.00