


Data Path : Z:\HPCHEM1\BNA G\Data\BG041218\
 Data File : BG033773.D
 Acq On : 12 Apr 2018 15:30
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 10 16:51:36 2018

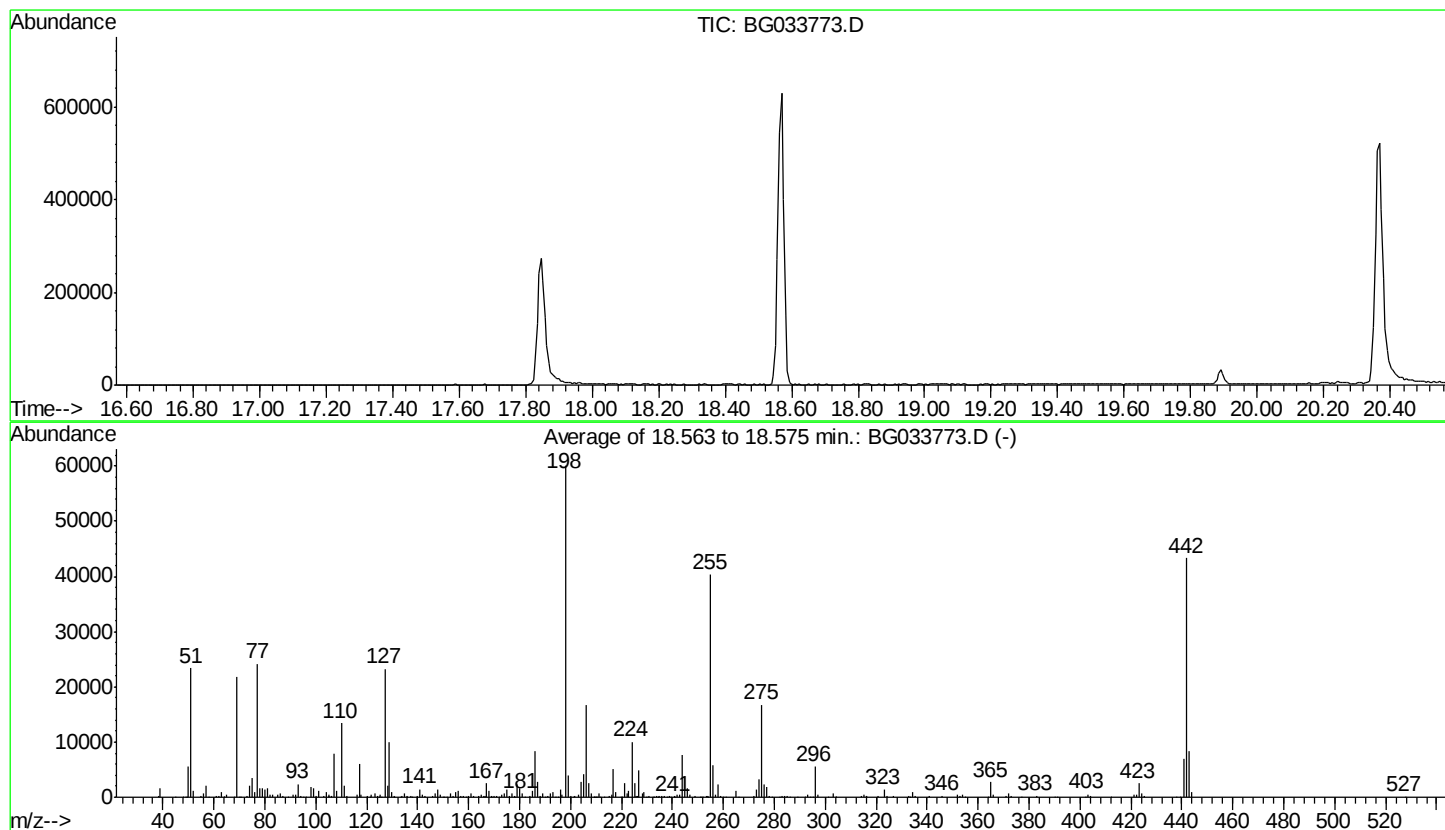

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	23354	PASS
68	69	0.00	2	0.4	96	PASS
69	198	0.00	100	36.3	21805	PASS
70	69	0.00	2	0.2	54	PASS
127	198	10	80	38.7	23229	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60064	PASS
199	198	5	9	6.7	3998	PASS
275	198	10	60	28.0	16802	PASS
365	198	1	100	4.6	2753	PASS
441	443	0.01	100	84.6	7061	PASS
442	198	50	100	72.0	43272	PASS
443	442	15	24	19.3	8351	PASS