
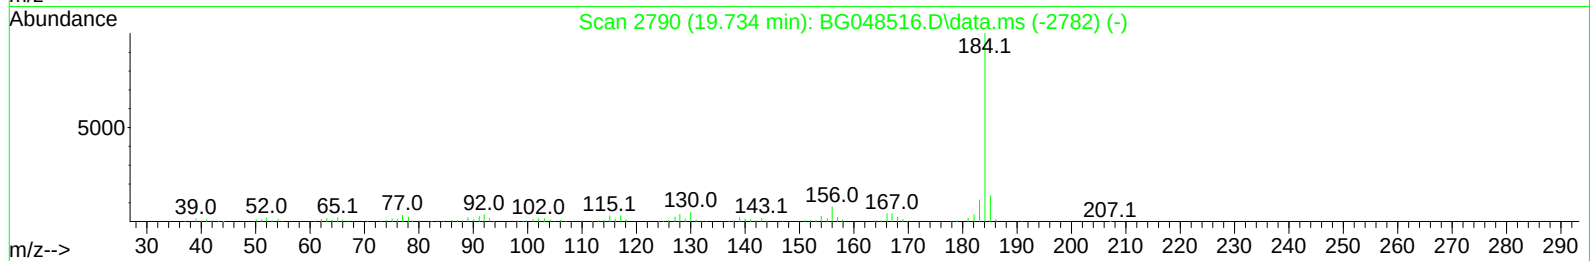
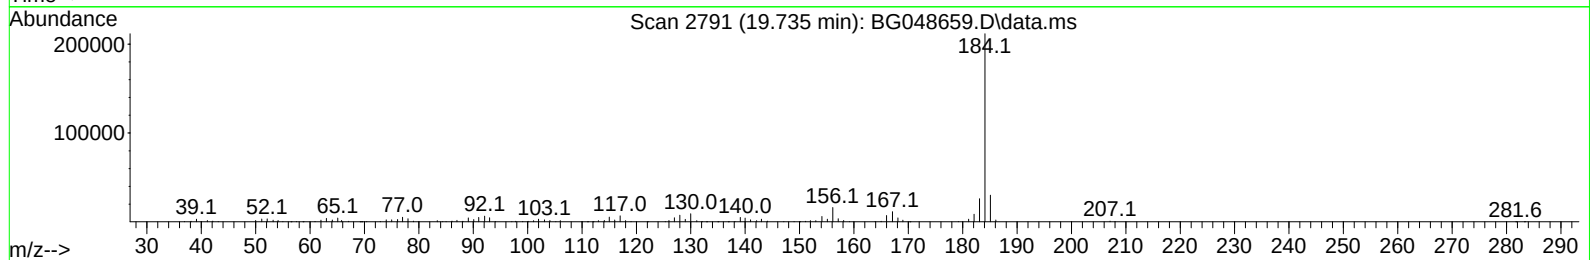


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041221\
Data File : BG048659.D
Acq On : 12 Apr 2021 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 11:02:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

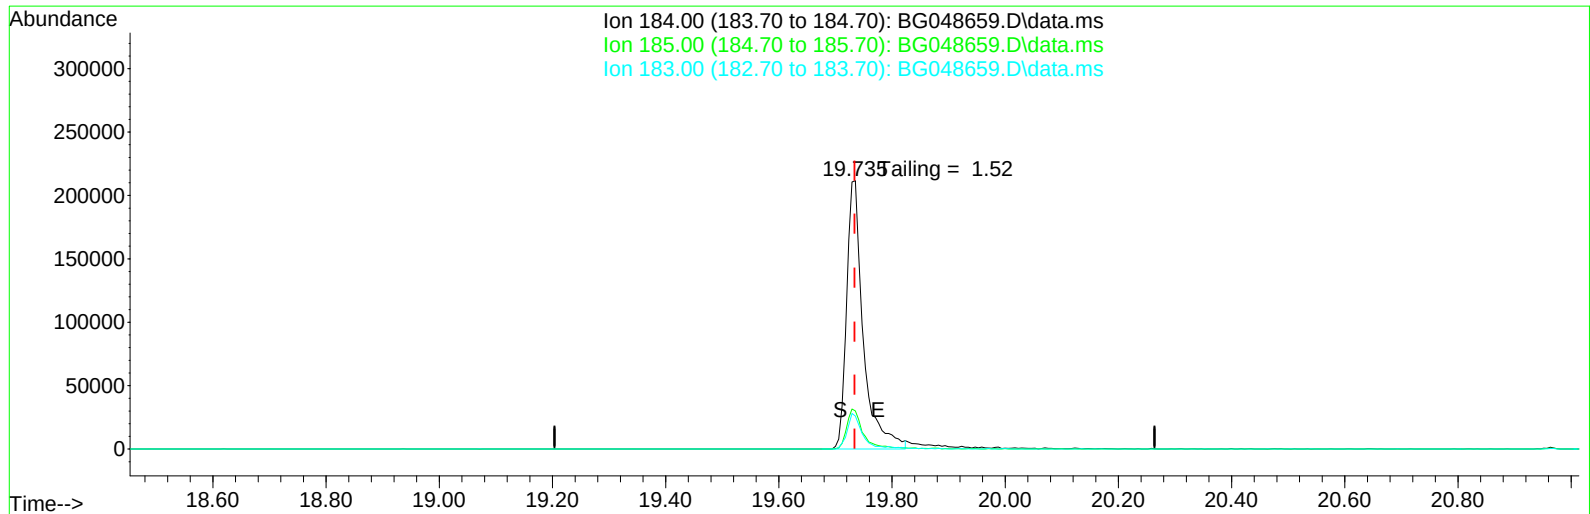




TIC: BG048659.D\data.ms

(77) Benzidine**19.735min (+ 0.002) 232785.66 ng****response 449321**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.18
183.00	11.50	12.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041221\
Data File : BG048659.D
Acq On : 12 Apr 2021 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 11:02:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

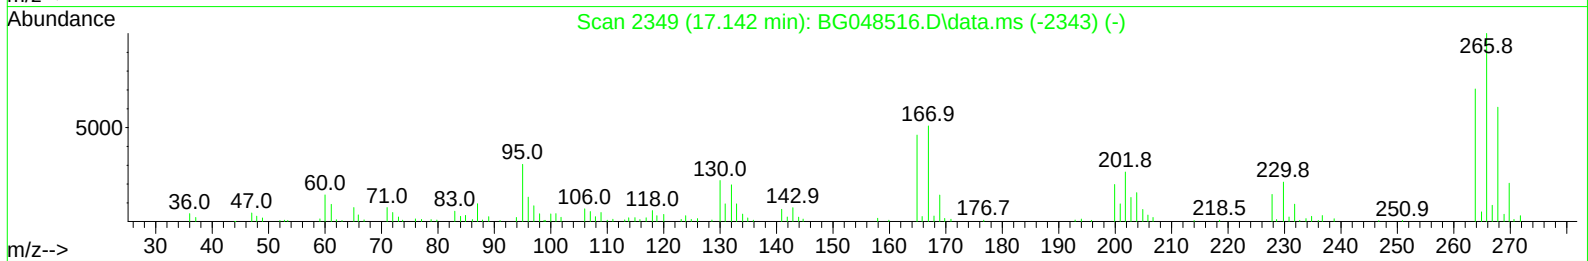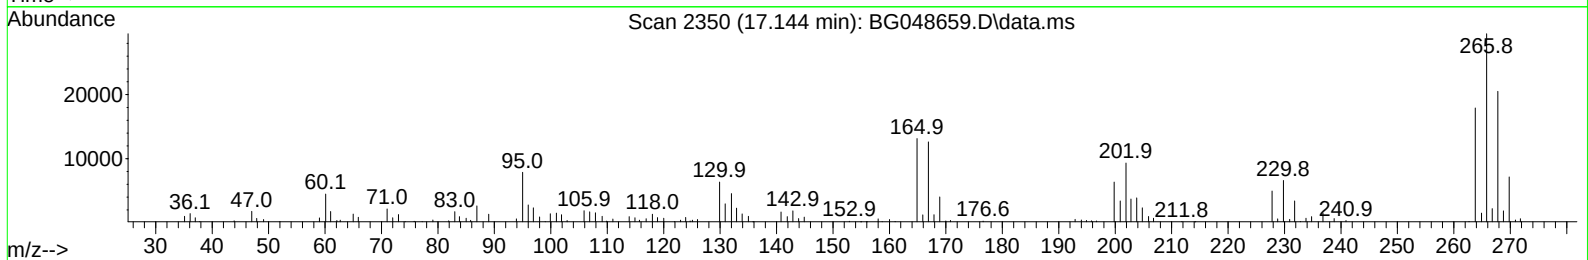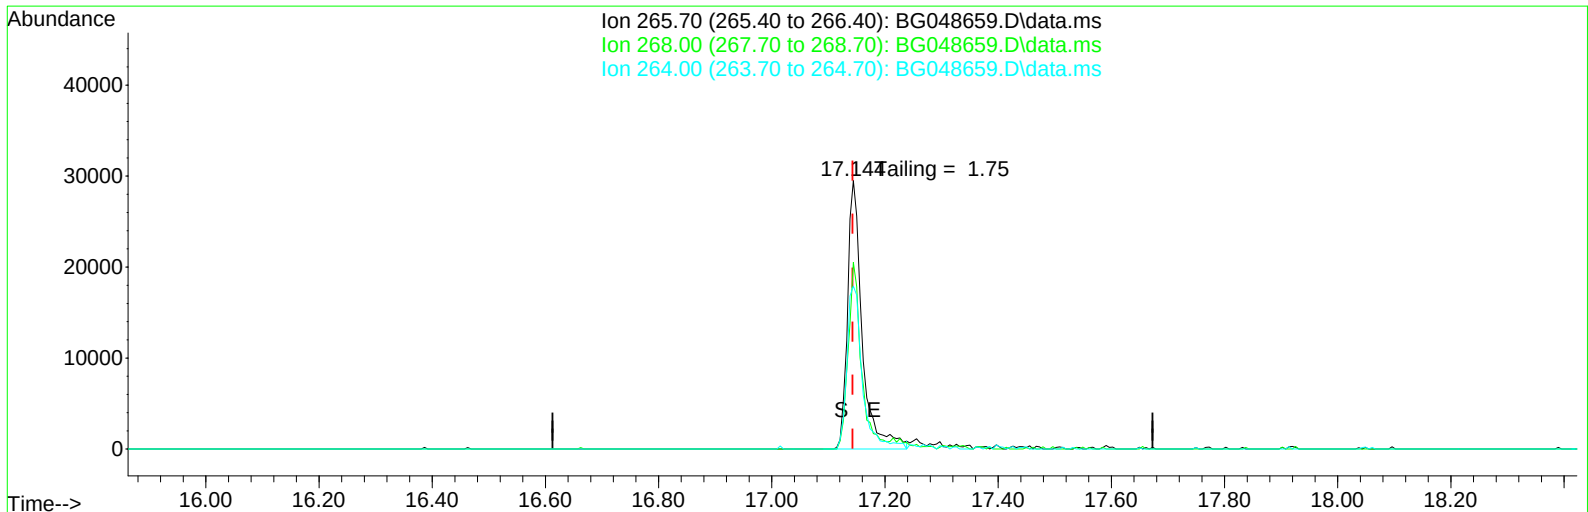

TIC: BG048659.D\data.ms

(70) Pentachlorophenol (C)

17.144min (+ 0.002) 18213.69 ng

response 53724

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	69.55
264.00	70.50	60.71
0.00	0.00	0.00