
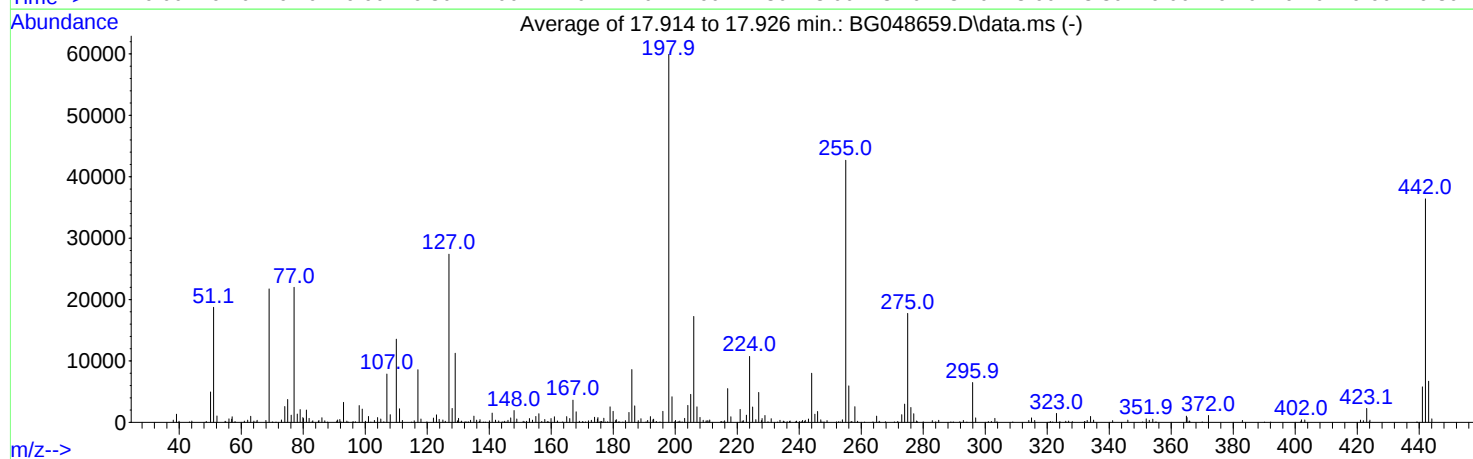


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041221\
 Data File : BG048659.D
 Acq On : 12 Apr 2021 10:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 07 10:06:00 2021

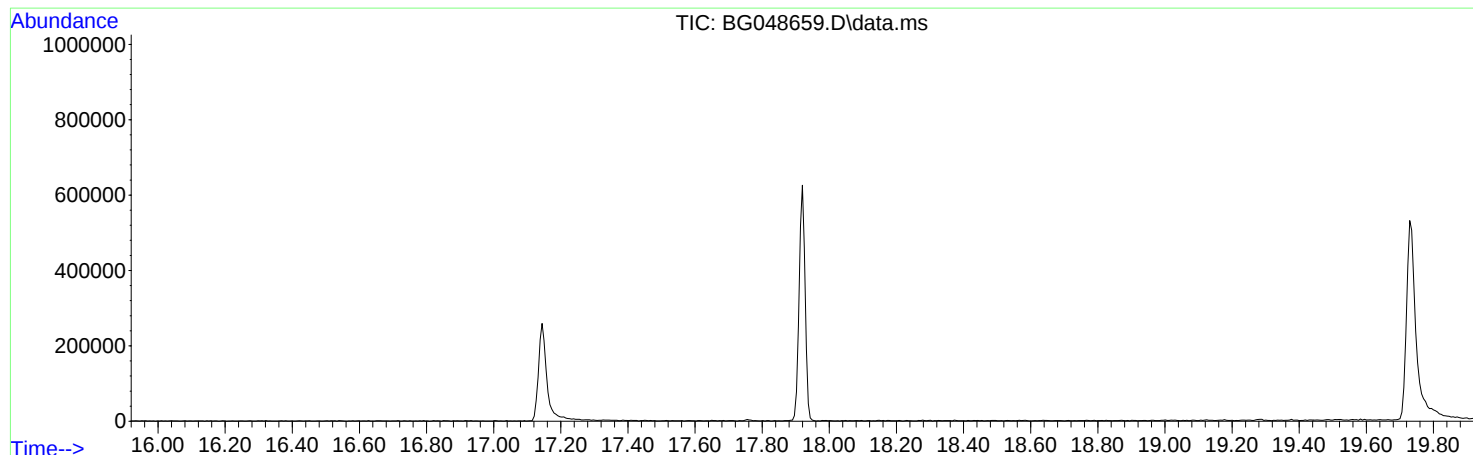




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	18735	PASS
68	69	0.00	2	1.5	323	PASS
69	198	0.00	100	36.3	21723	PASS
70	69	0.00	2	0.3	62	PASS
127	198	10	80	45.7	27400	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59909	PASS
199	198	5	9	7.0	4171	PASS
275	198	10	60	29.6	17742	PASS
365	198	1	100	1.7	1011	PASS
441	198	0.01	100	9.7	5792	PASS
442	198	50	100	60.8	36411	PASS
443	442	15	24	18.4	6689	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041221\
Data File : BG048659.D
Acq On : 12 Apr 2021 10:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 12 11:02:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

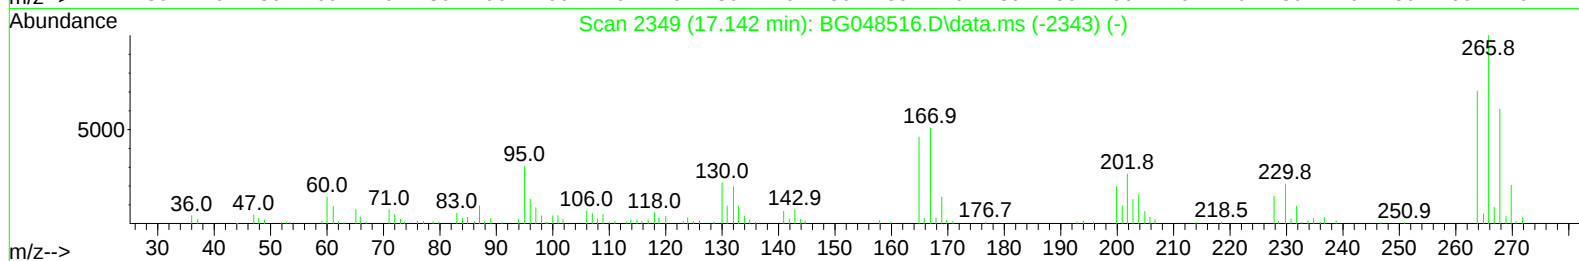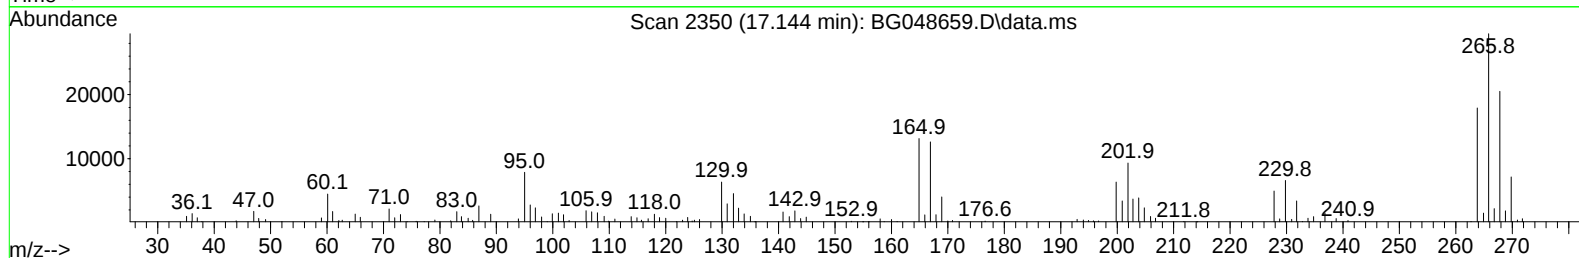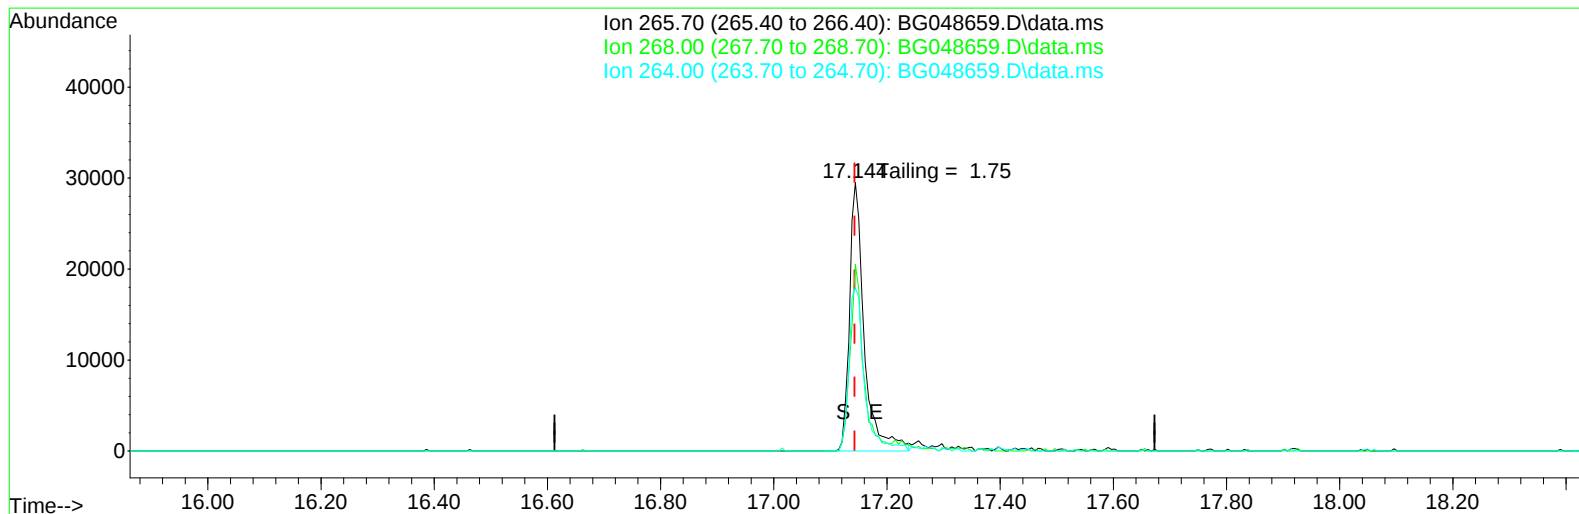

TIC: BG048659.D\data.ms

(70) Pentachlorophenol (C)

17.144min (+ 0.002) 18213.69 ng

response 53724

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	69.55
264.00	70.50	60.71
0.00	0.00	0.00

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/12/2021	BNA_G	<u>BG048659.D</u>
Compound Name	Response	Retention Time
DDT	251495	20.96
DDD	1091	20.56
DDE	388	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1479	252974	0.58