
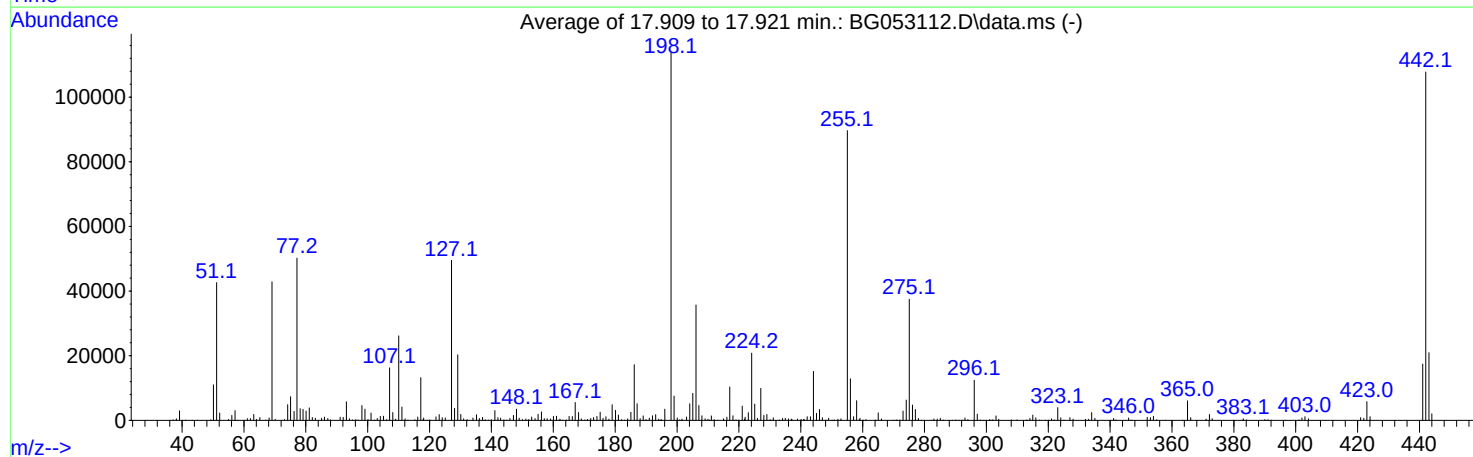


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041222\
 Data File : BG053112.D
 Acq On : 12 Apr 2022 9:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 15:31:24 2022

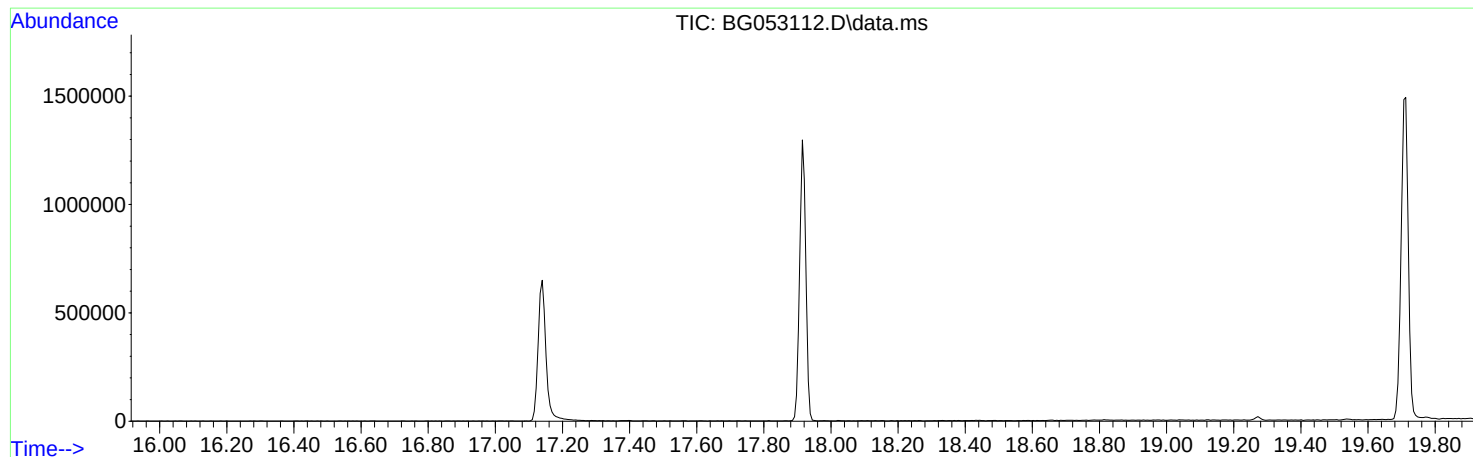




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	42624	PASS
68	69	0.00	2	1.7	728	PASS
69	198	0.00	100	37.7	42880	PASS
70	69	0.00	2	0.7	287	PASS
127	198	10	80	43.5	49499	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	113808	PASS
199	198	5	9	6.6	7544	PASS
275	198	10	60	32.9	37491	PASS
365	198	1	100	5.3	6065	PASS
441	198	0.01	100	15.3	17437	PASS
442	442	50	100	100.0	107789	PASS
443	442	15	24	19.4	20925	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041222\
Data File : BG053112.D
Acq On : 12 Apr 2022 9:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 13 08:59:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

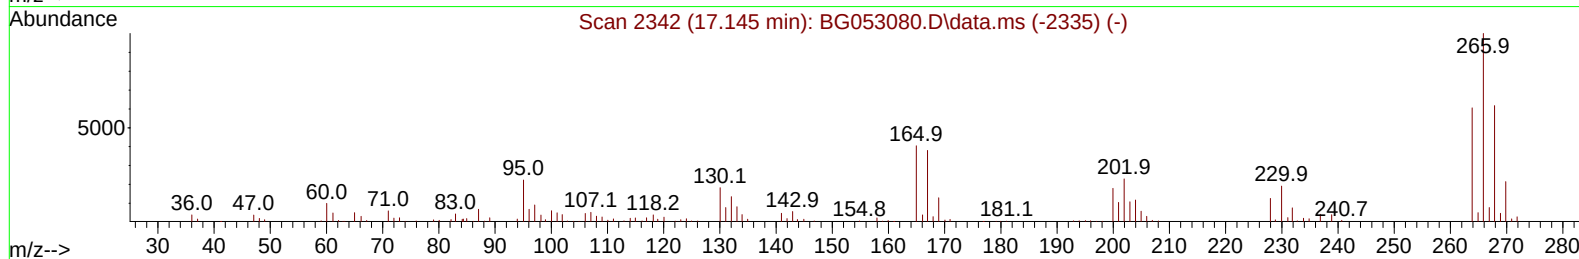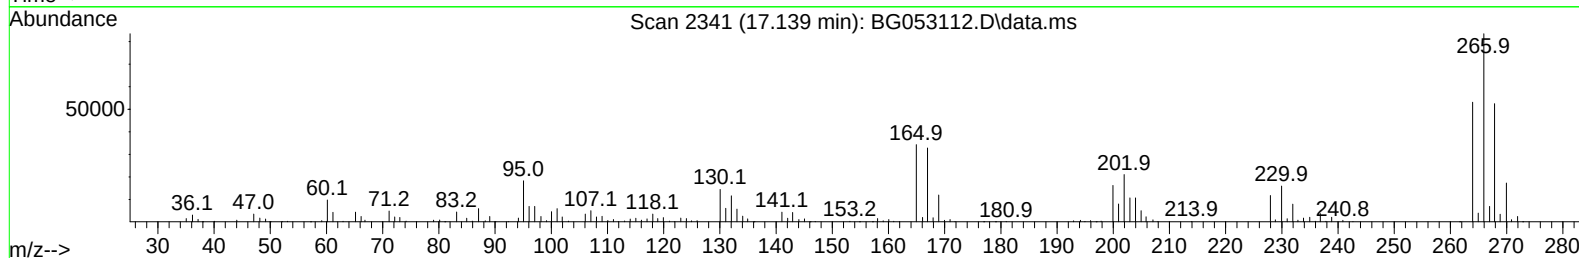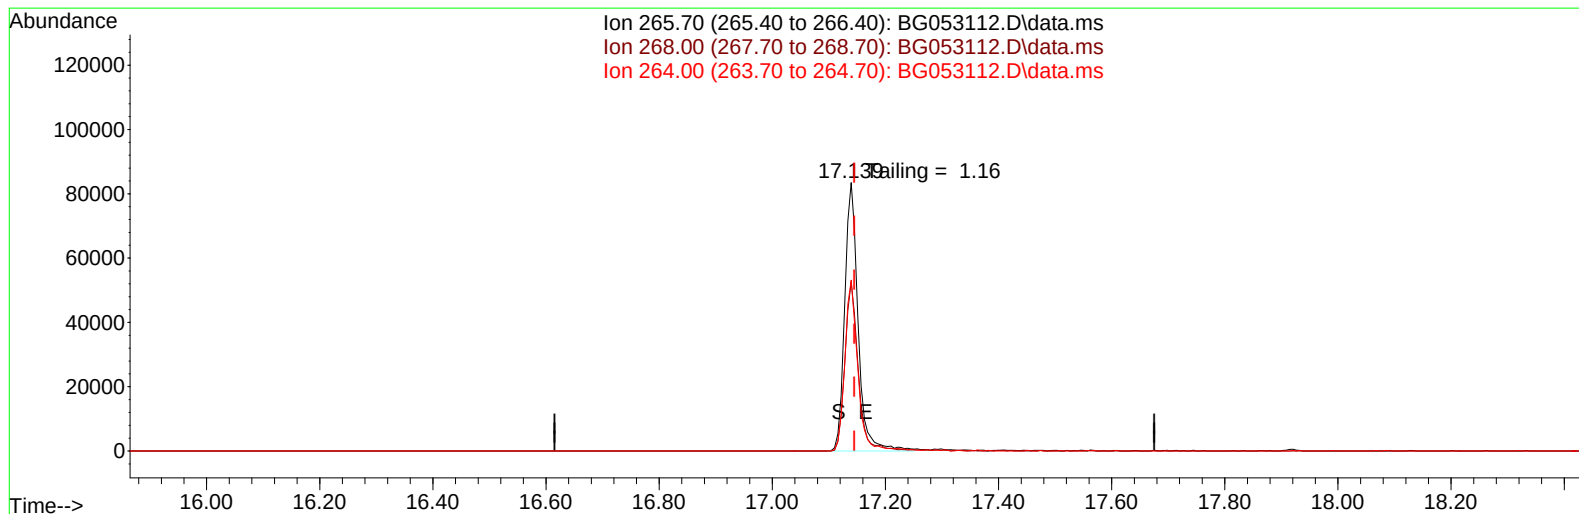

TIC: BG053112.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.006) 0.00 ng




response 138562

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	62.92
264.00	56.60	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041222\
Data File : BG053112.D
Acq On : 12 Apr 2022 9:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 13 08:59:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

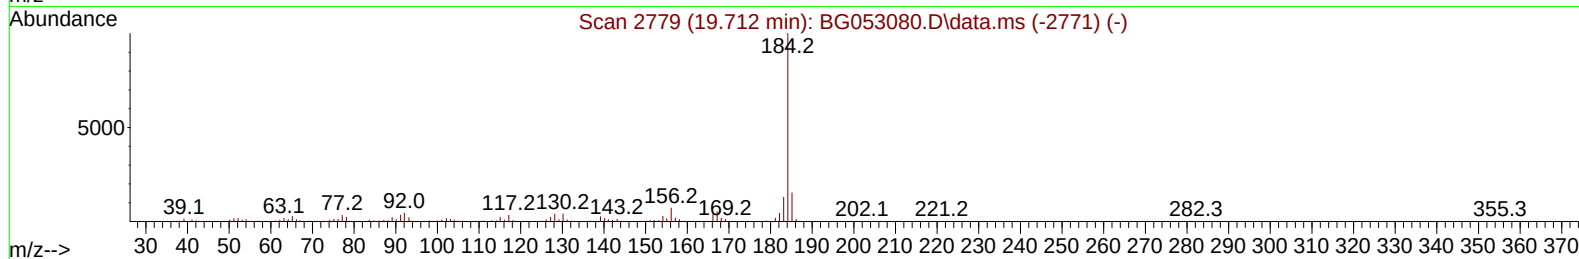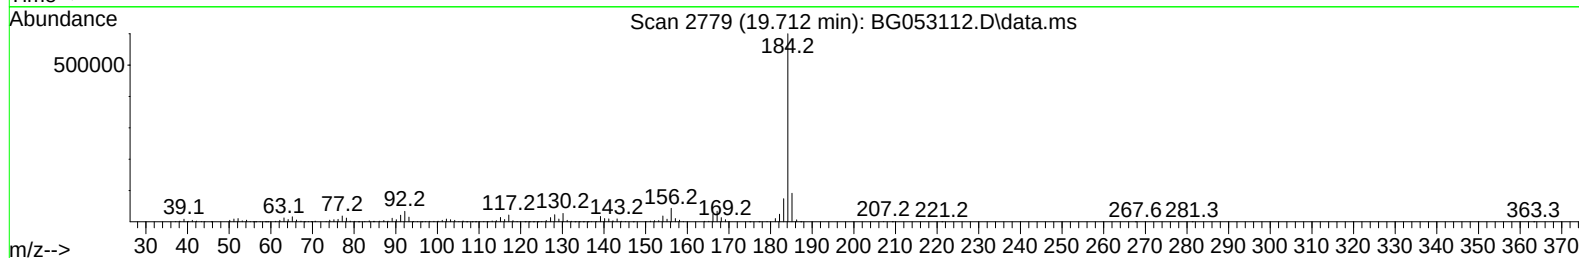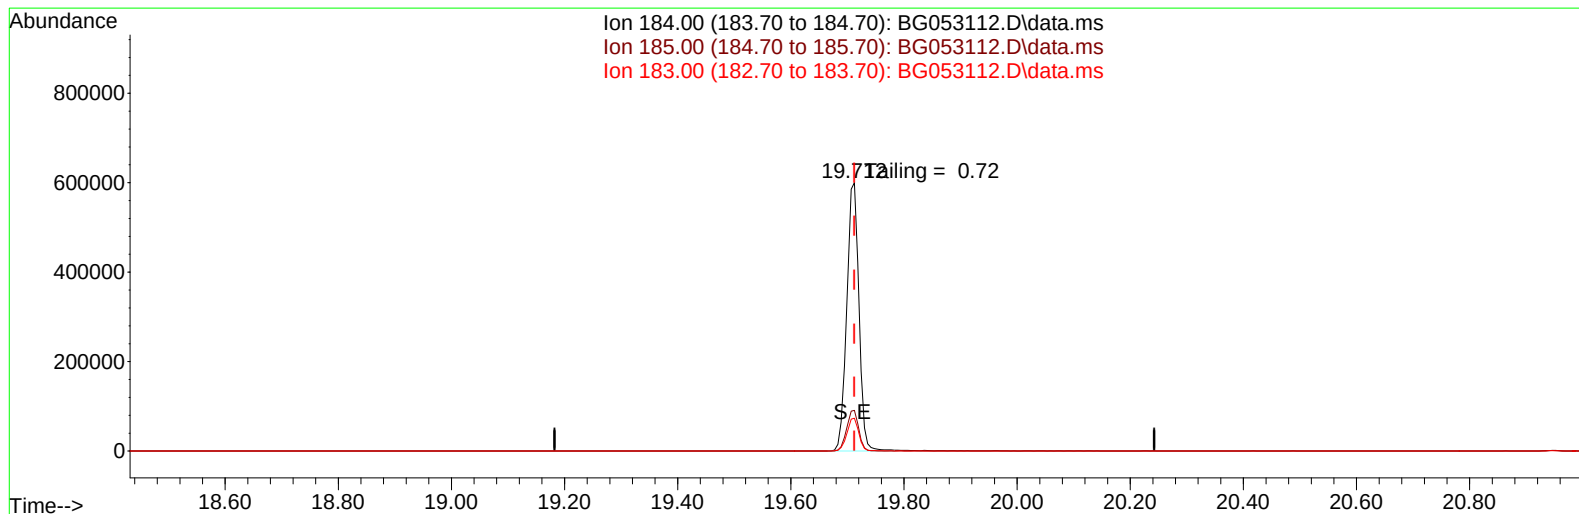

TIC: BG053112.D\data.ms

(77) Benzidine

19.712min (+ 0.000) 244590.79 ng

response 900235

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.18
183.00	11.80	12.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/12/2022	BNA_G	<u>BG053112.D</u>
Compound Name	Response	Retention Time
DDT	453562	20.946
DDD	5170	20.5
DDE	534	19.994
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5704	459266	1.24

Instrument :
BNA_G
ClientSampleId :
DFTPP