
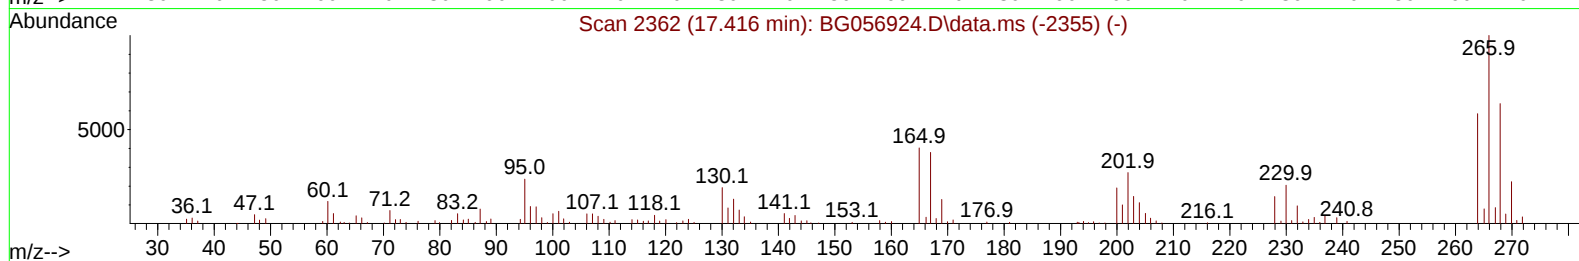
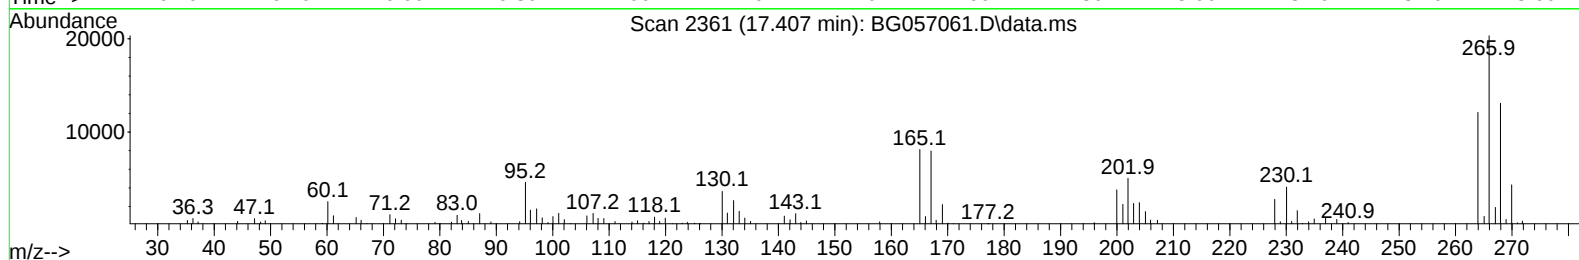


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041223\
Data File : BG057061.D
Acq On : 12 Apr 2023 12:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 06:45:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:15:23 2023
Response via : Initial Calibration

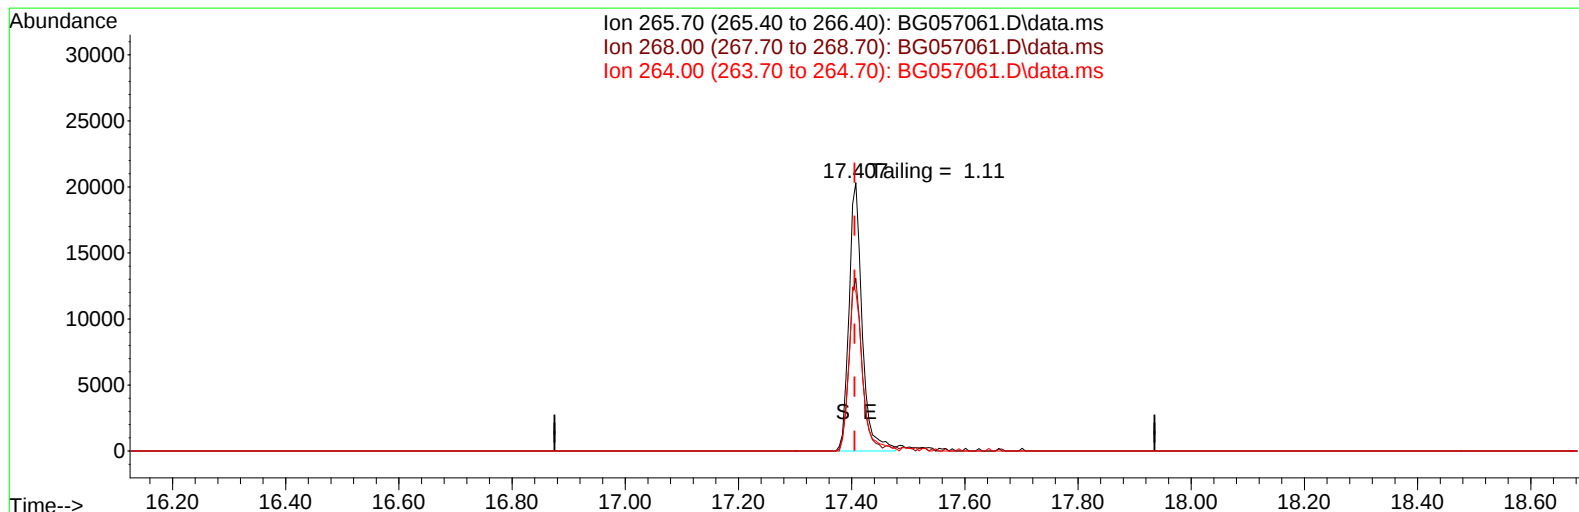

TIC: BG057061.D\data.ms

(70) Pentachlorophenol (C)




17.407min (+ 0.003) 28856.66 ng

response 32922

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.33
264.00	58.50	59.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041223\
Data File : BG057061.D
Acq On : 12 Apr 2023 12:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 06:45:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:15:23 2023
Response via : Initial Calibration

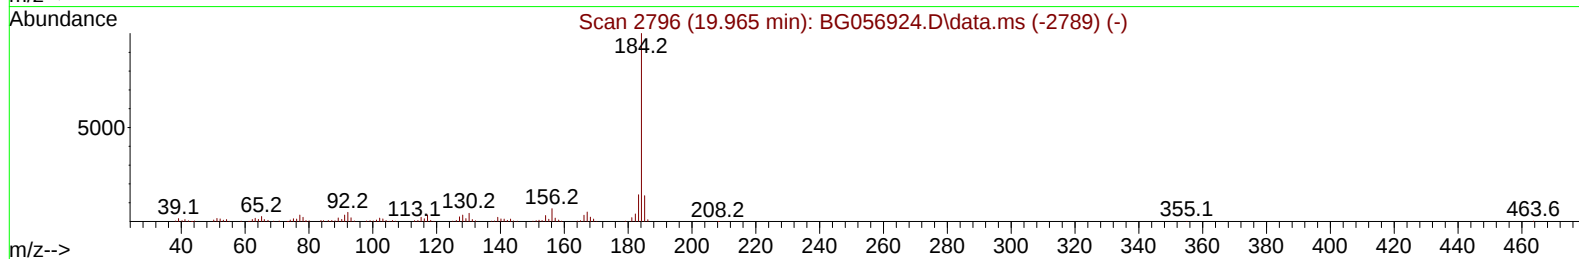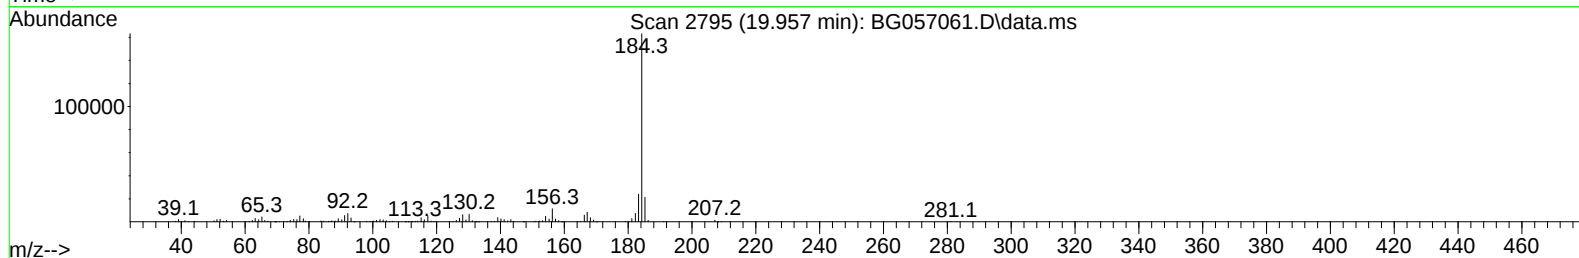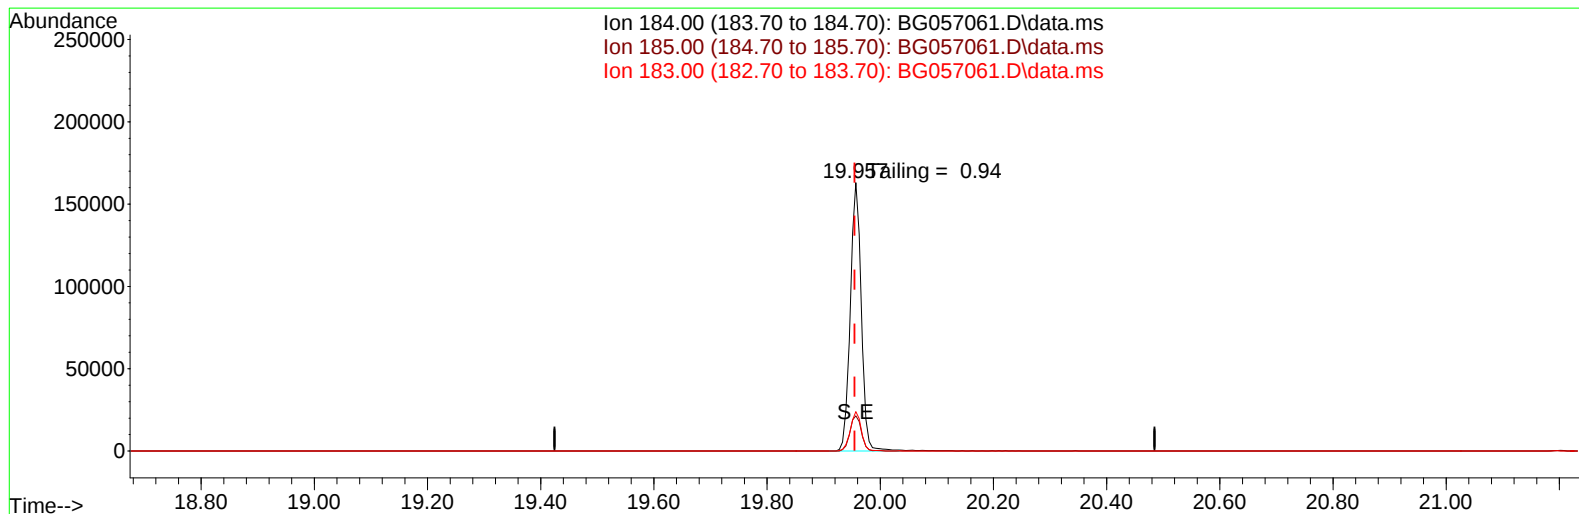

TIC: BG057061.D\data.ms

(77) Benzidine

19.957min (+ 0.003) 0.00 ng

response 219963

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.12
183.00	14.20	14.70
0.00	0.00	0.00