


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041223\
 Data File : BG057061.D
 Acq On : 12 Apr 2023 12:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 13 05:15:23 2023

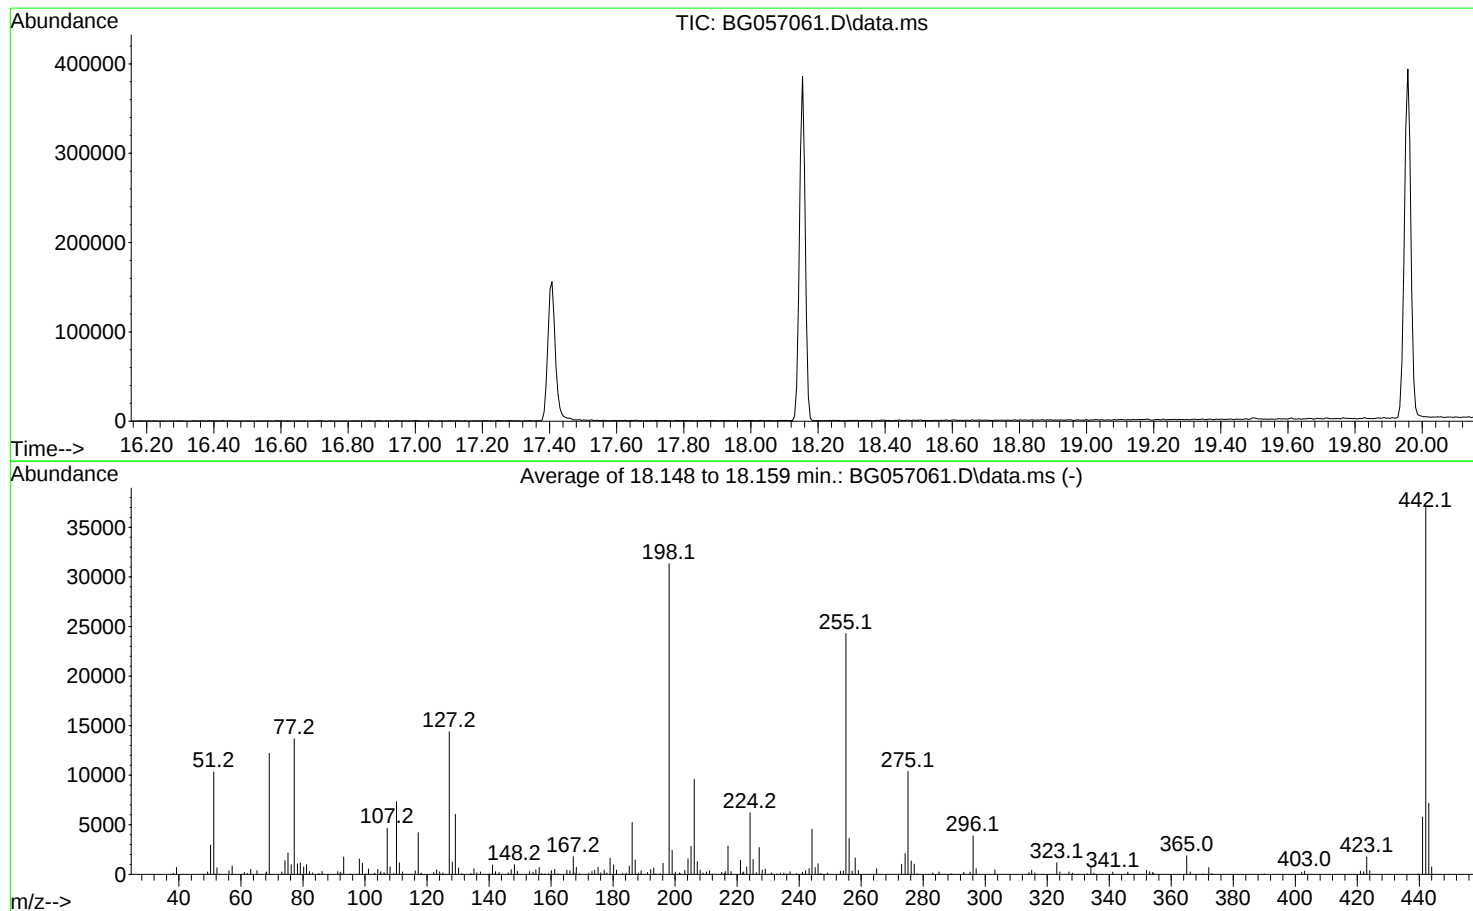

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	10334	PASS
68	69	0.00	2	2.0	243	PASS
69	198	0.00	100	38.9	12207	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.9	14382	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31347	PASS
199	198	5	9	7.7	2422	PASS
275	198	10	60	33.1	10375	PASS
365	198	1	100	6.0	1877	PASS
441	198	0.01	100	18.5	5787	PASS
442	442	50	100	100.0	37104	PASS
443	442	15	24	19.3	7167	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/12/2023	BNA_G	<u>BG057061.D</u>
Compound Name	Response	Retention Time
DDT	112133	21.196
DDD	3412	20.732
DDE	145	20.233
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3557	115690	3.07

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041223\
Data File : BG057061.D
Acq On : 12 Apr 2023 12:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 13 06:45:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:15:23 2023
Response via : Initial Calibration

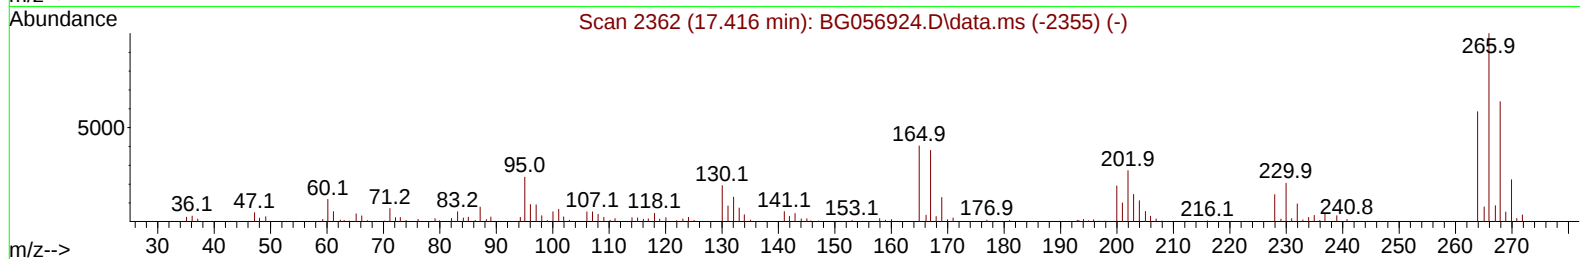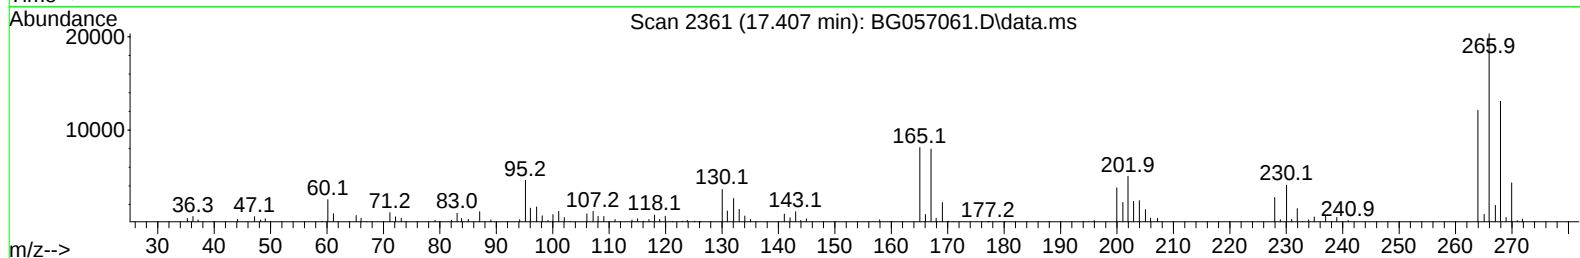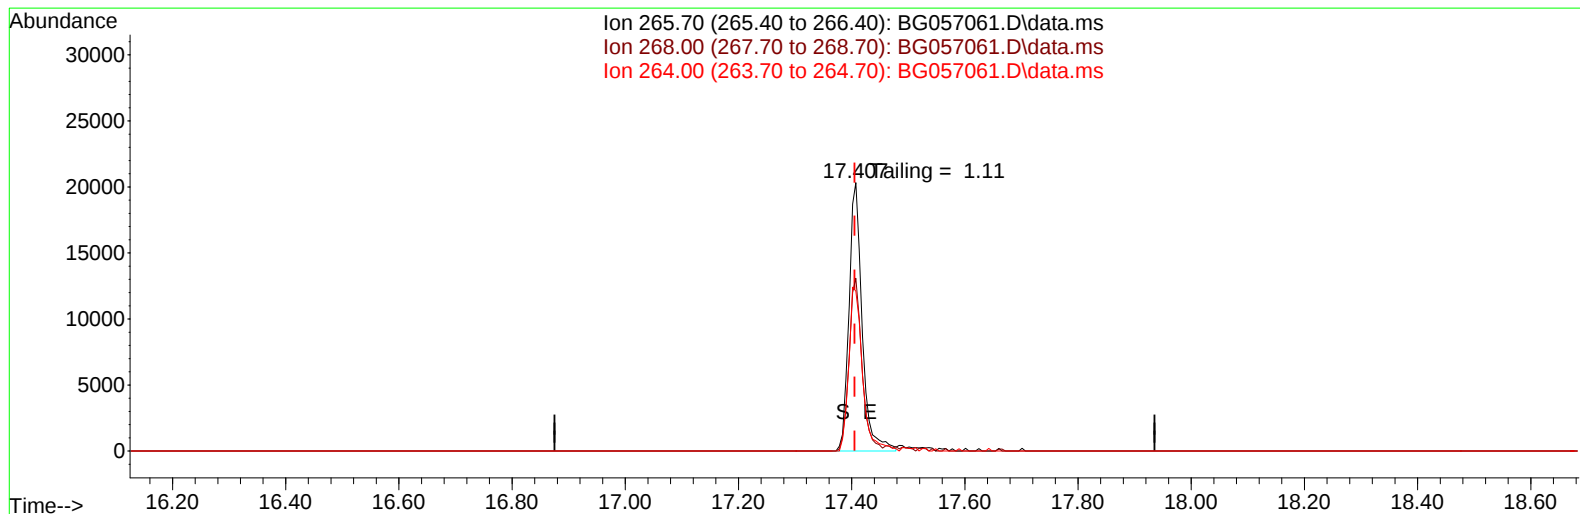

TIC: BG057061.D\data.ms

(70) Pentachlorophenol (C)

17.407min (+ 0.003) 28856.66 ng




response 32922

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.33
264.00	58.50	59.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041223\
Data File : BG057061.D
Acq On : 12 Apr 2023 12:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 13 06:45:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:15:23 2023
Response via : Initial Calibration

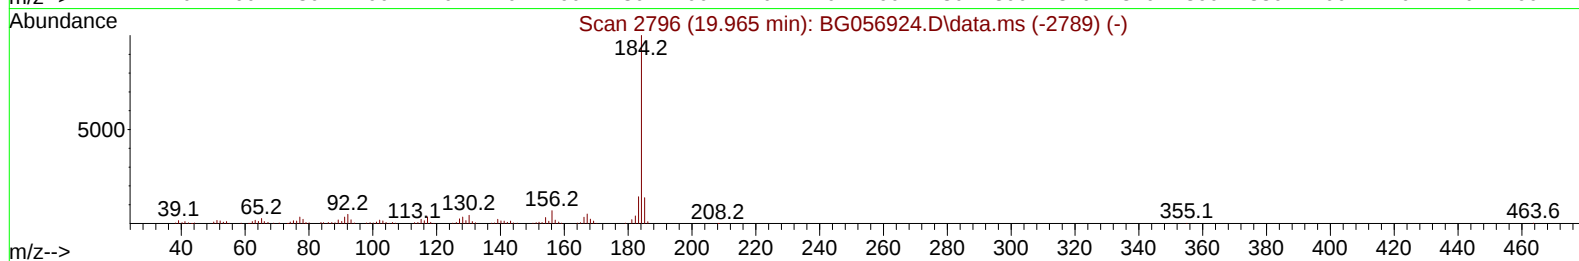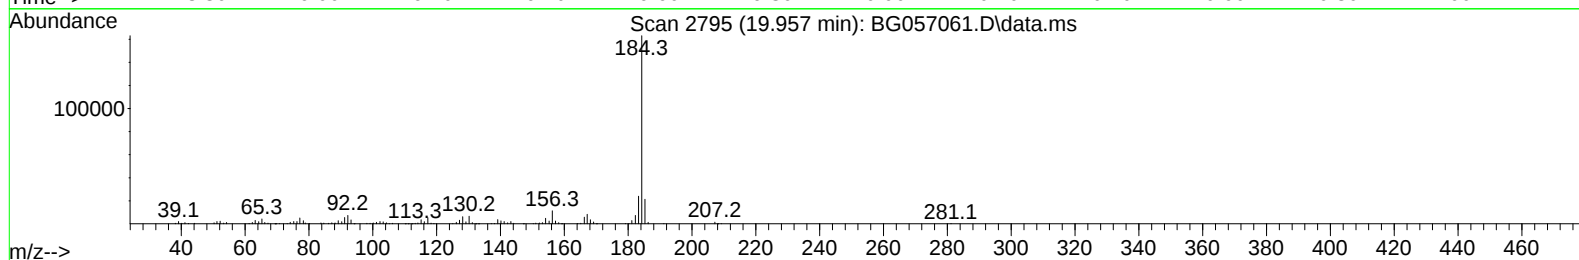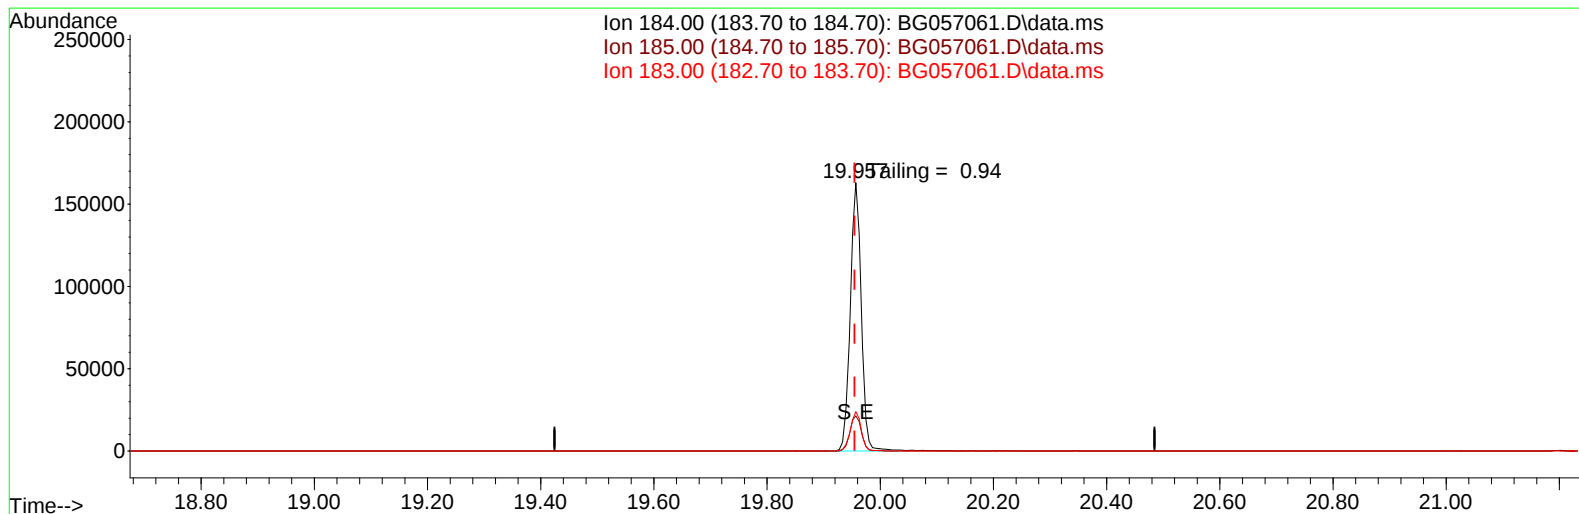

TIC: BG057061.D\data.ms

(77) Benzidine

19.957min (+ 0.003) 0.00 ng

response 219963

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.12
183.00	14.20	14.70
0.00	0.00	0.00