
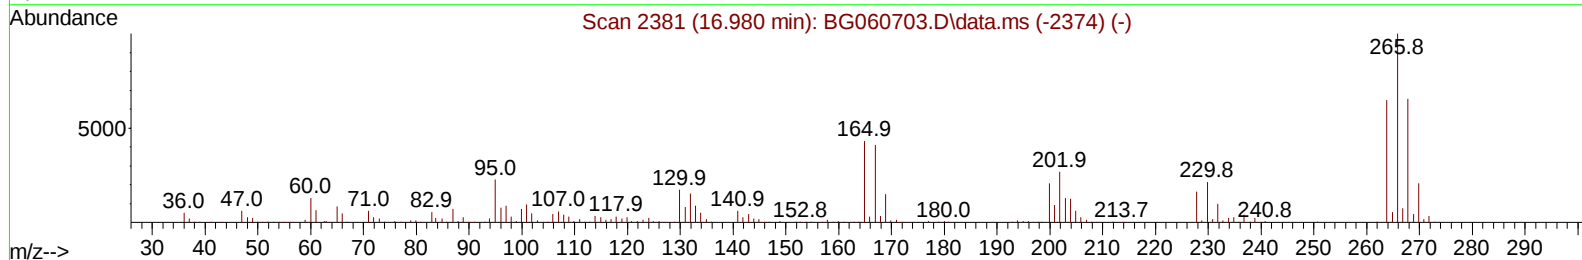
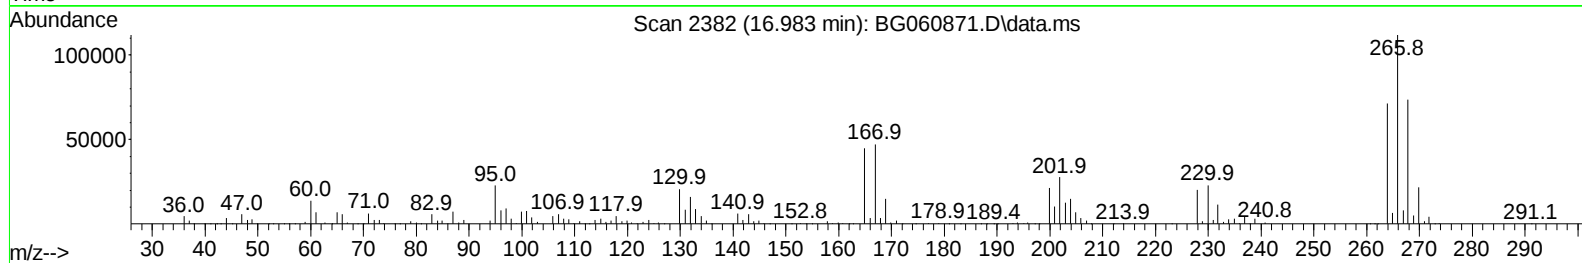


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041224\
Data File : BG060871.D
Acq On : 12 Apr 2024 11:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 12:11:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

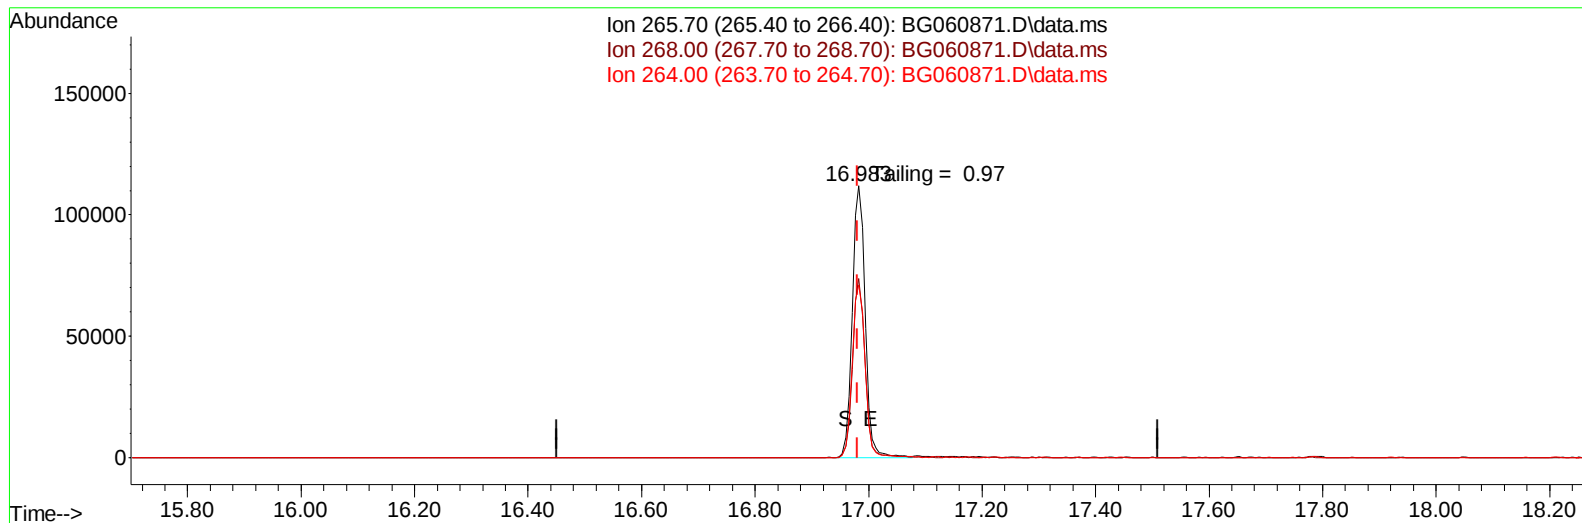




TIC: BG060871.D\data.ms

(70) Pentachlorophenol (C)**16.983min (+ 0.003) 22983.25 ng****response 174902**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.97
264.00	64.70	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041224\
Data File : BG060871.D
Acq On : 12 Apr 2024 11:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 12:11:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

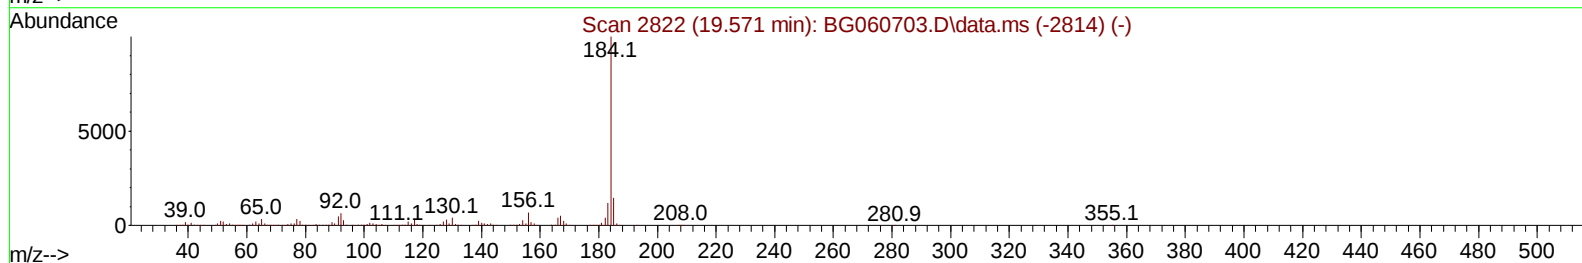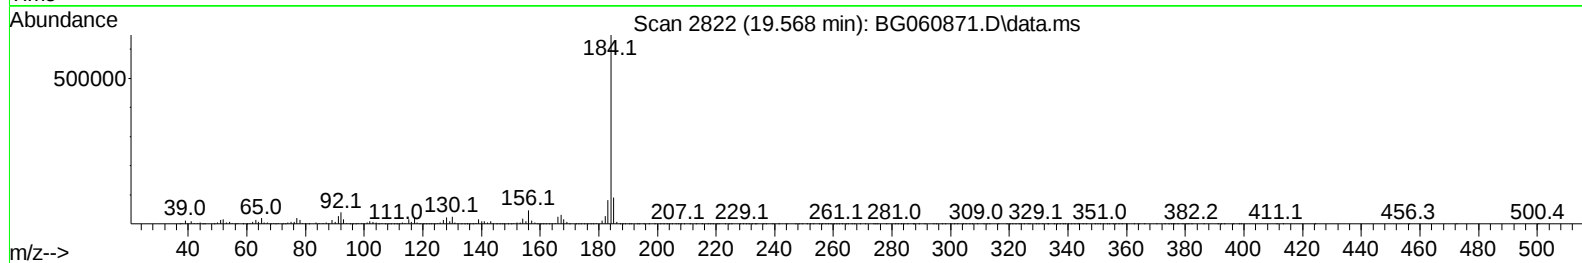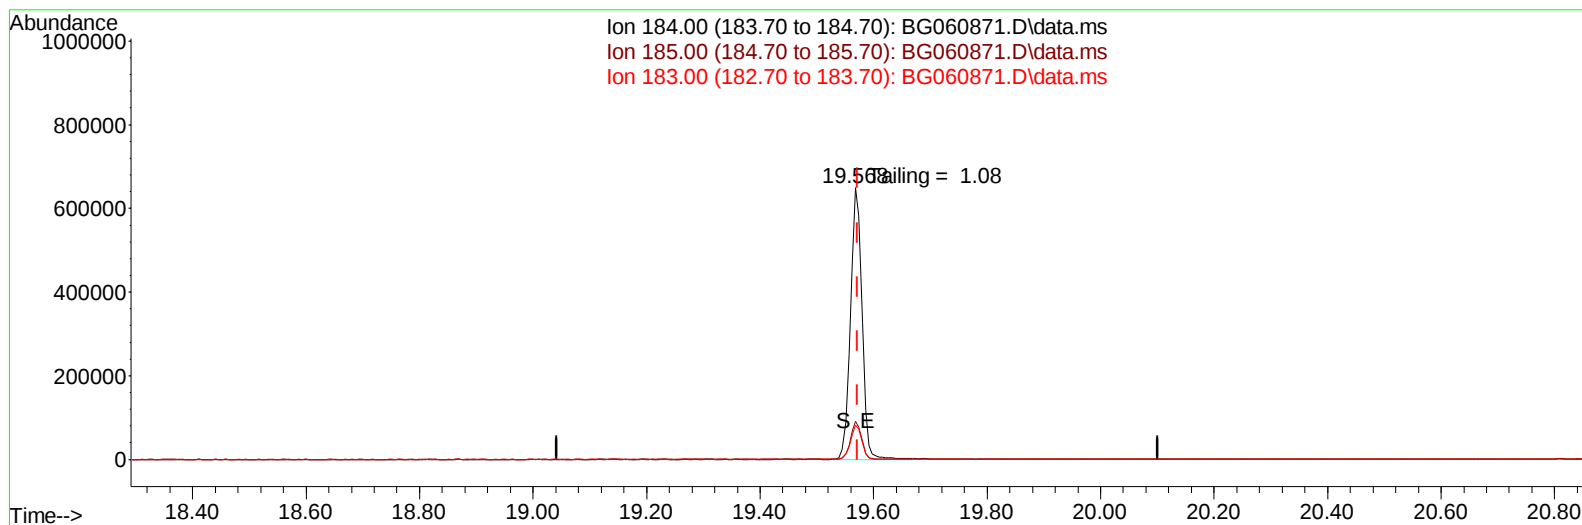

TIC: BG060871.D\data.ms

(77) Benzidine**19.568min (-0.003) 99031.22 ng****response 904874**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.98
183.00	11.90	12.73
0.00	0.00	0.00