


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041315\
 Data File : BG016376.D
 Acq On : 14 Apr 2015 1:24
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 07 04:17:17 2015

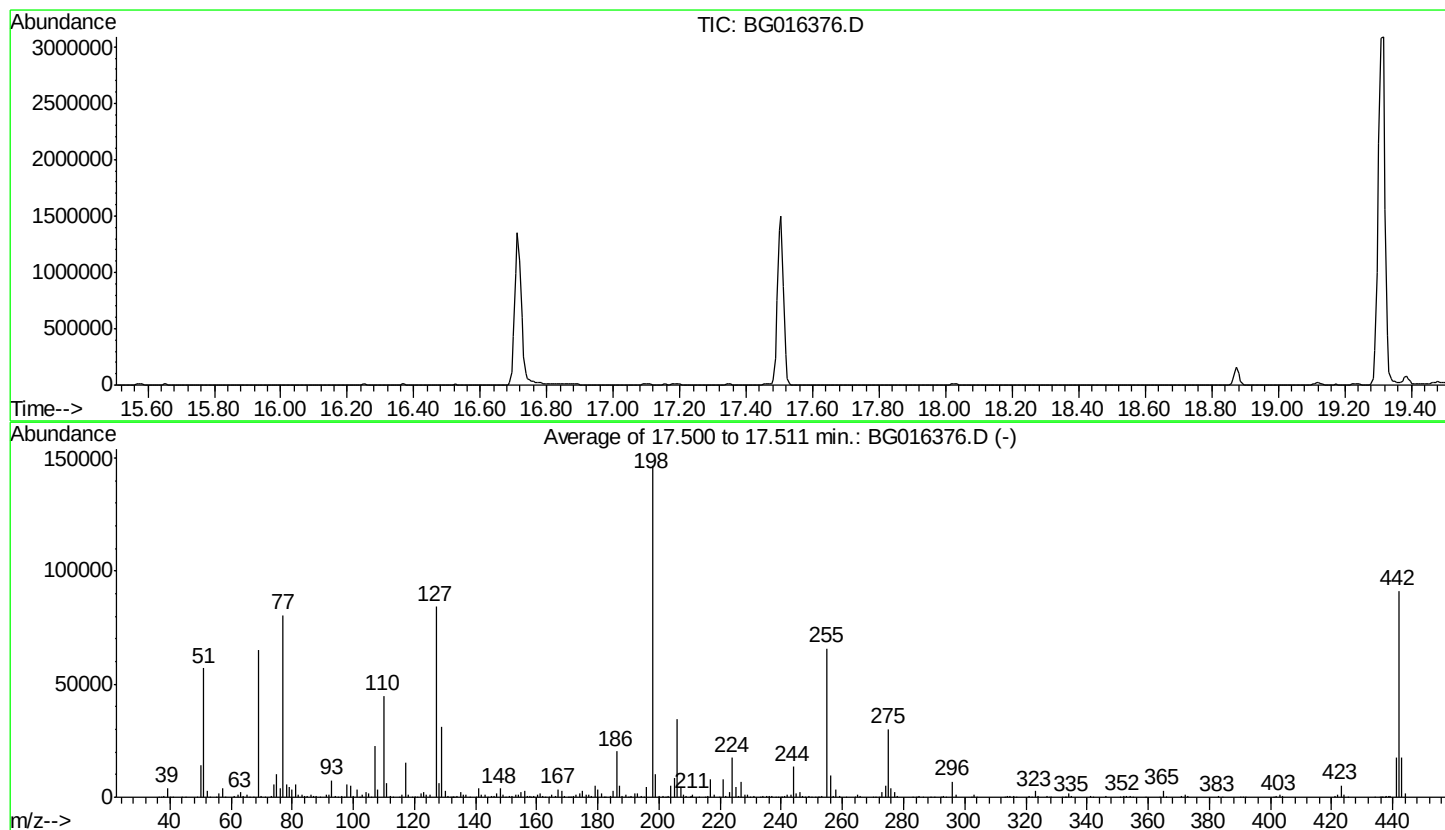

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	56965	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.5	65234	PASS
70	69	0.00	2	0.5	317	PASS
127	198	10	80	57.4	84197	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	146717	PASS
199	198	5	9	6.8	9963	PASS
275	198	10	60	20.6	30285	PASS
365	198	1	100	2.1	3012	PASS
441	442	0.01	24	19.2	17531	PASS
442	198	50	100	62.3	91333	PASS
443	442	15	24	19.5	17848	PASS