
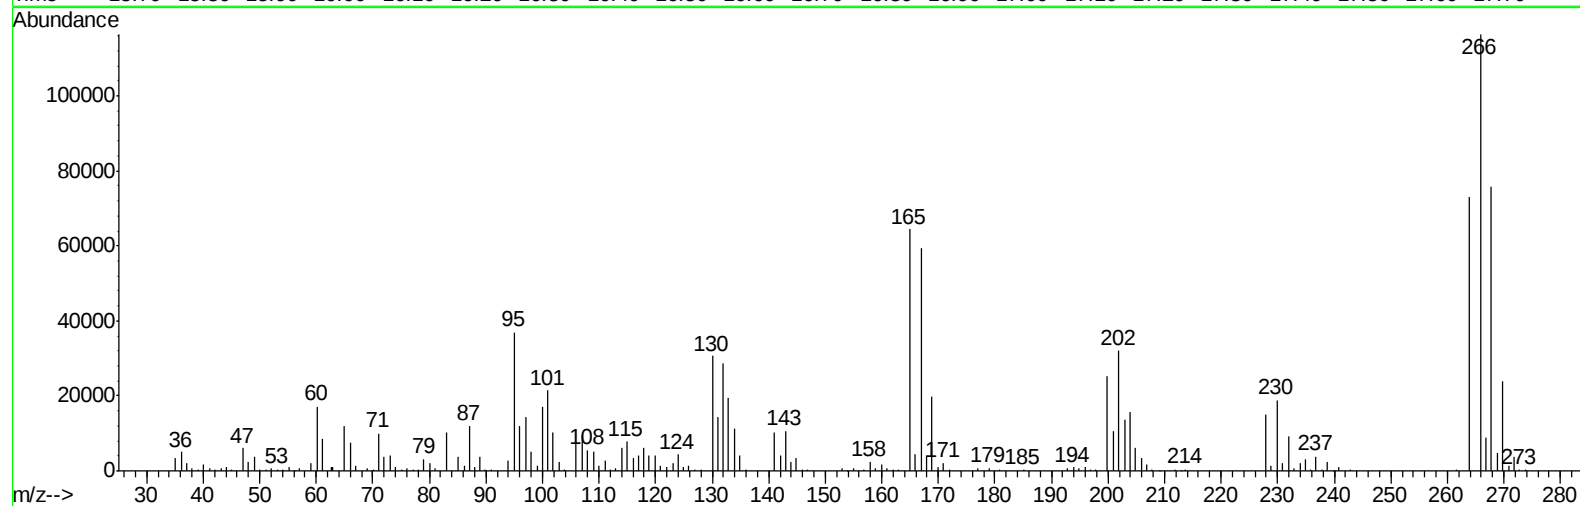


Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG041315\  
Data File : BG016358.D  
Acq On : 13 Apr 2015 13:03  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 07:38:41 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG040615.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 14 07:14:14 2015  
Response via : Initial Calibration

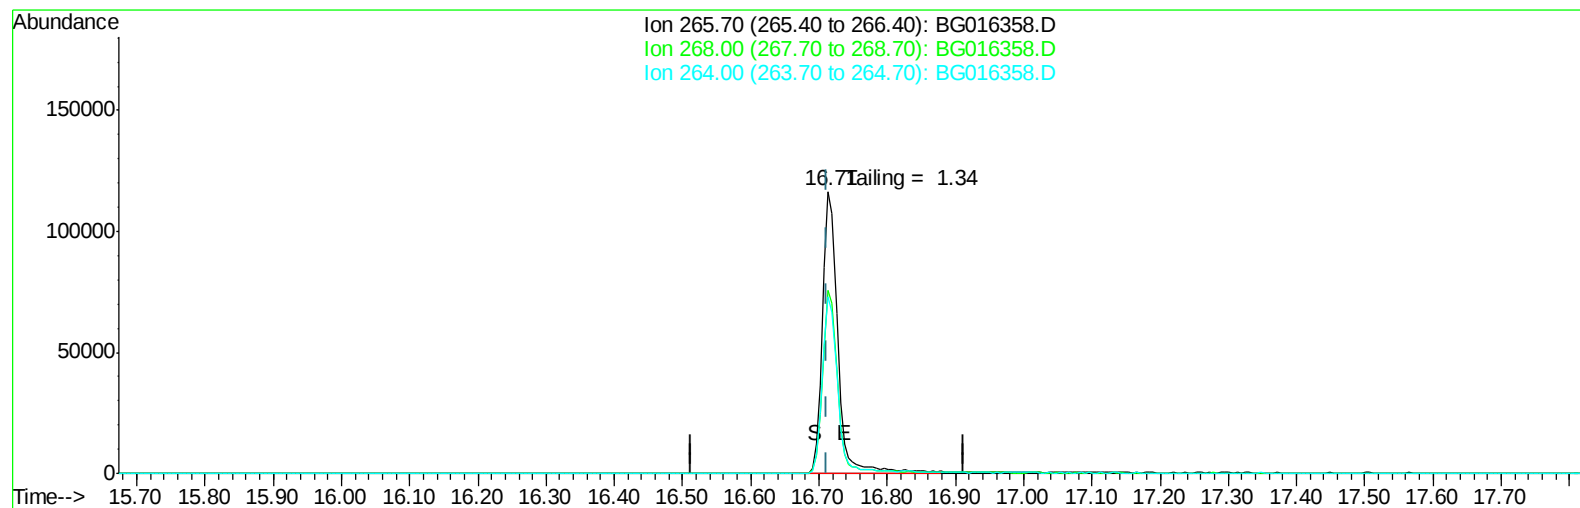

TIC: BG016358.D

(69) Pentachlorophenol (C)



16.714min (+0.001) 59601.39ng

response 178187

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.60 | 65.21 |
| 264.00 | 66.00 | 62.65 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG041315\  
Data File : BG016358.D  
Acq On : 13 Apr 2015 13:03  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 07:38:41 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG040615.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 14 07:14:14 2015  
Response via : Initial Calibration

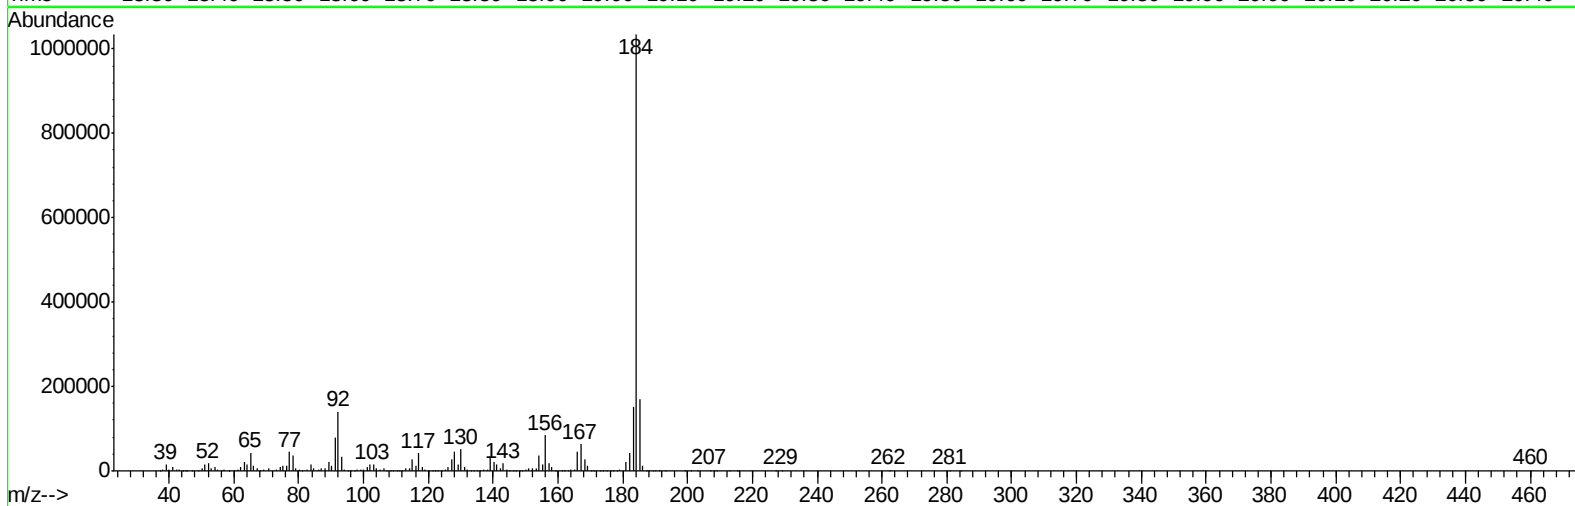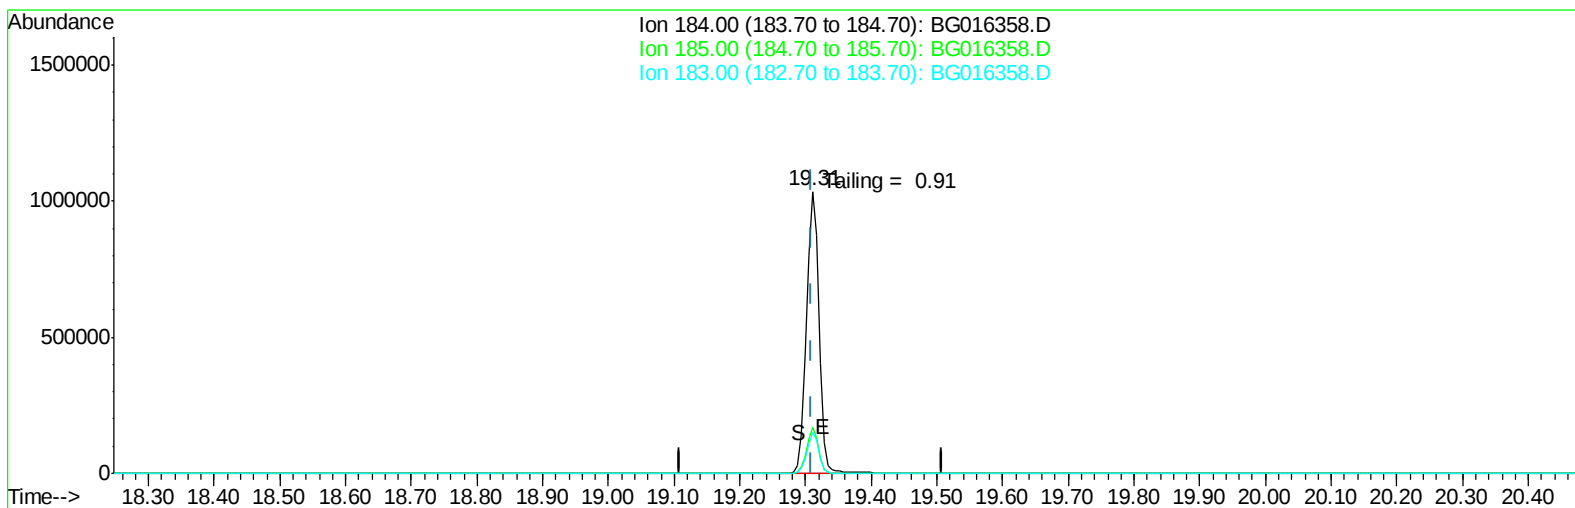

TIC: BG016358.D

(76) Benzidine

19.311min (+0.001) 26869.12ng m

response 1376454

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.80 | 16.36 |
| 183.00 | 13.00 | 14.56 |
| 0.00   | 0.00  | 0.00  |