
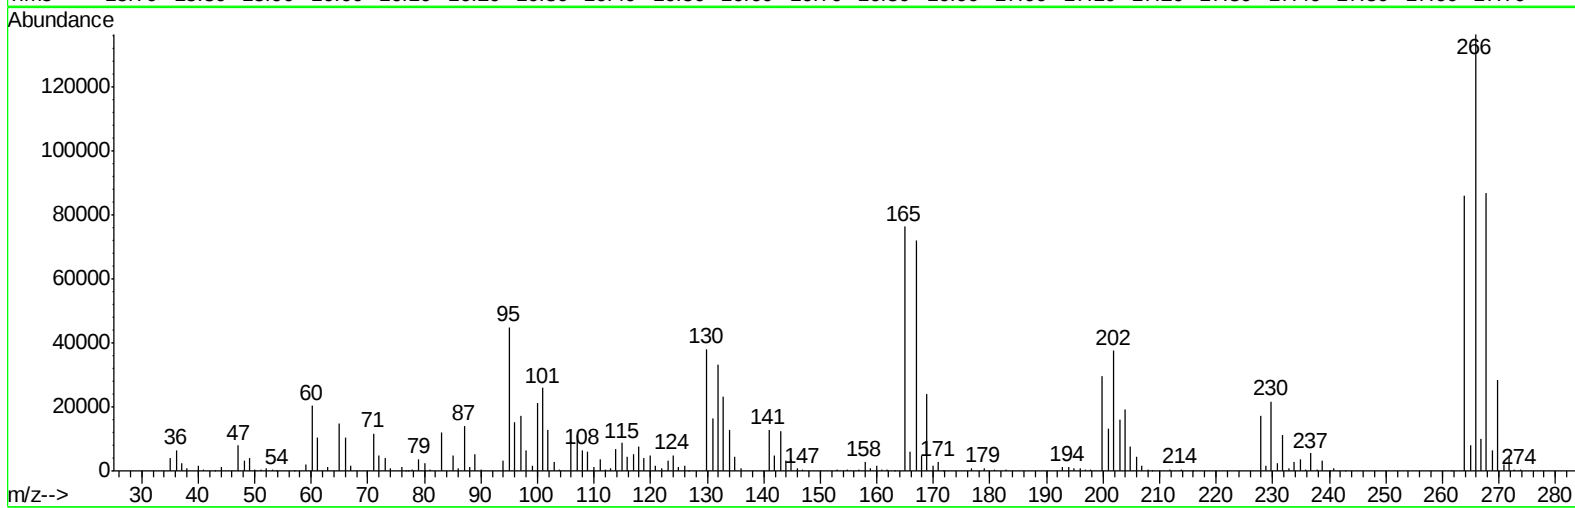


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041315\
Data File : BG016376.D
Acq On : 14 Apr 2015 1:24
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 07:39:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 07:14:14 2015
Response via : Initial Calibration

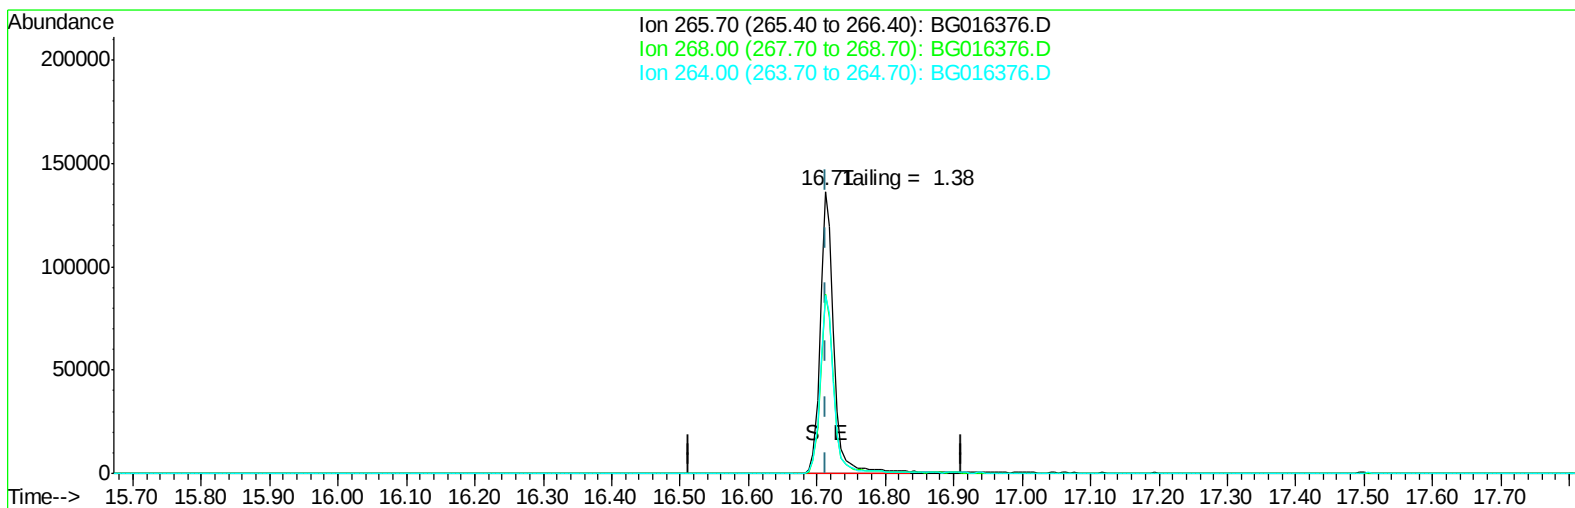

TIC: BG016376.D

(69) Pentachlorophenol (C)



16.712min (-0.000) 38156.33ng

response 189672

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.63
264.00	66.00	63.18
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041315\
Data File : BG016376.D
Acq On : 14 Apr 2015 1:24
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 07:39:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 07:14:14 2015
Response via : Initial Calibration

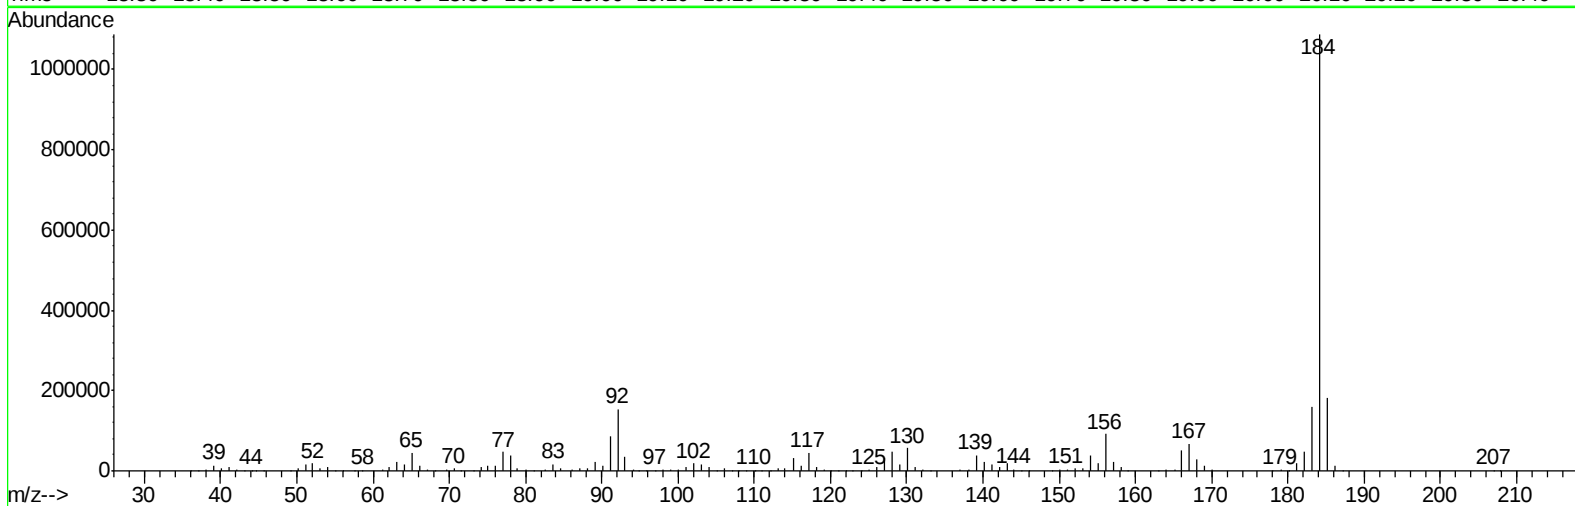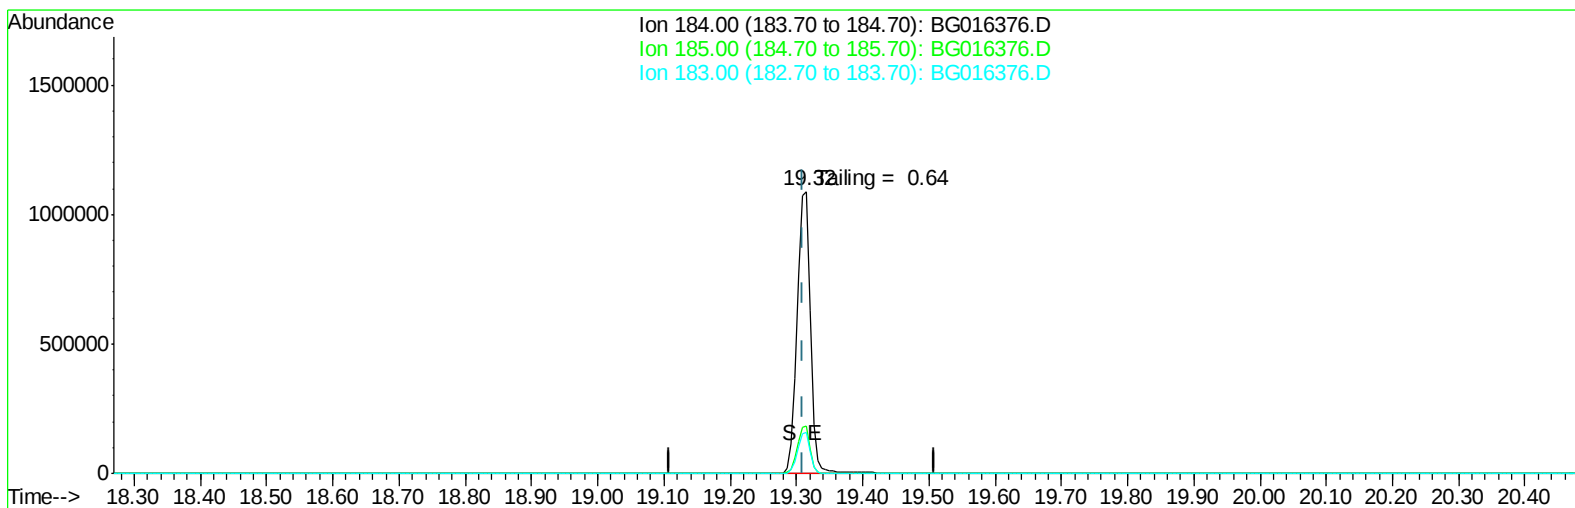

TIC: BG016376.D

(76) Benzidine

19.315min (+0.005) 22564.29ng

response 1553993

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.77
183.00	13.00	14.76
0.00	0.00	0.00