

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041315\
 Data File : BG016383.D
 Acq On : 14 Apr 2015 6:02
 Operator : TP/IZ
 Sample : G1851-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FS-027

Quant Time: Apr 14 07:28:19 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 14 07:14:14 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	80968	20.00	ng	0.00
21) Naphthalene-d8	10.46	136	349046	20.00	ng	0.00
38) Acenaphthene-d10	14.32	164	189445	20.00	ng	0.00
63) Phenanthrene-d10	17.05	188	391920	20.00	ng	0.00
75) Chrysene-d12	21.23	240	361112	20.00	ng	0.00
86) Perylene-d12	23.47	264	339803	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	610735	119.04	ng	0.00
7) Phenol-d6	6.86	99	859758	111.63	ng	0.00
23) Nitrobenzene-d5	8.83	82	450649	74.79	ng	0.00
41) 2,4,6-Tribromophenol	15.81	330	163351	127.50	ng	0.00
44) 2-Fluorobiphenyl	12.94	172	889269	79.92	ng	0.00
78) Terphenyl-d14	19.69	244	1039015	67.34	ng	0.00
Target Compounds						
49) Dimethylphthalate	13.78	163	95576	6.88	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041315\
Data File : BG016383.D
Acq On : 14 Apr 2015 6:02
Operator : TP/IZ
Sample : G1851-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FS-027

Quant Time: Apr 14 07:28:19 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 07:14:14 2015
Response via : Initial Calibration

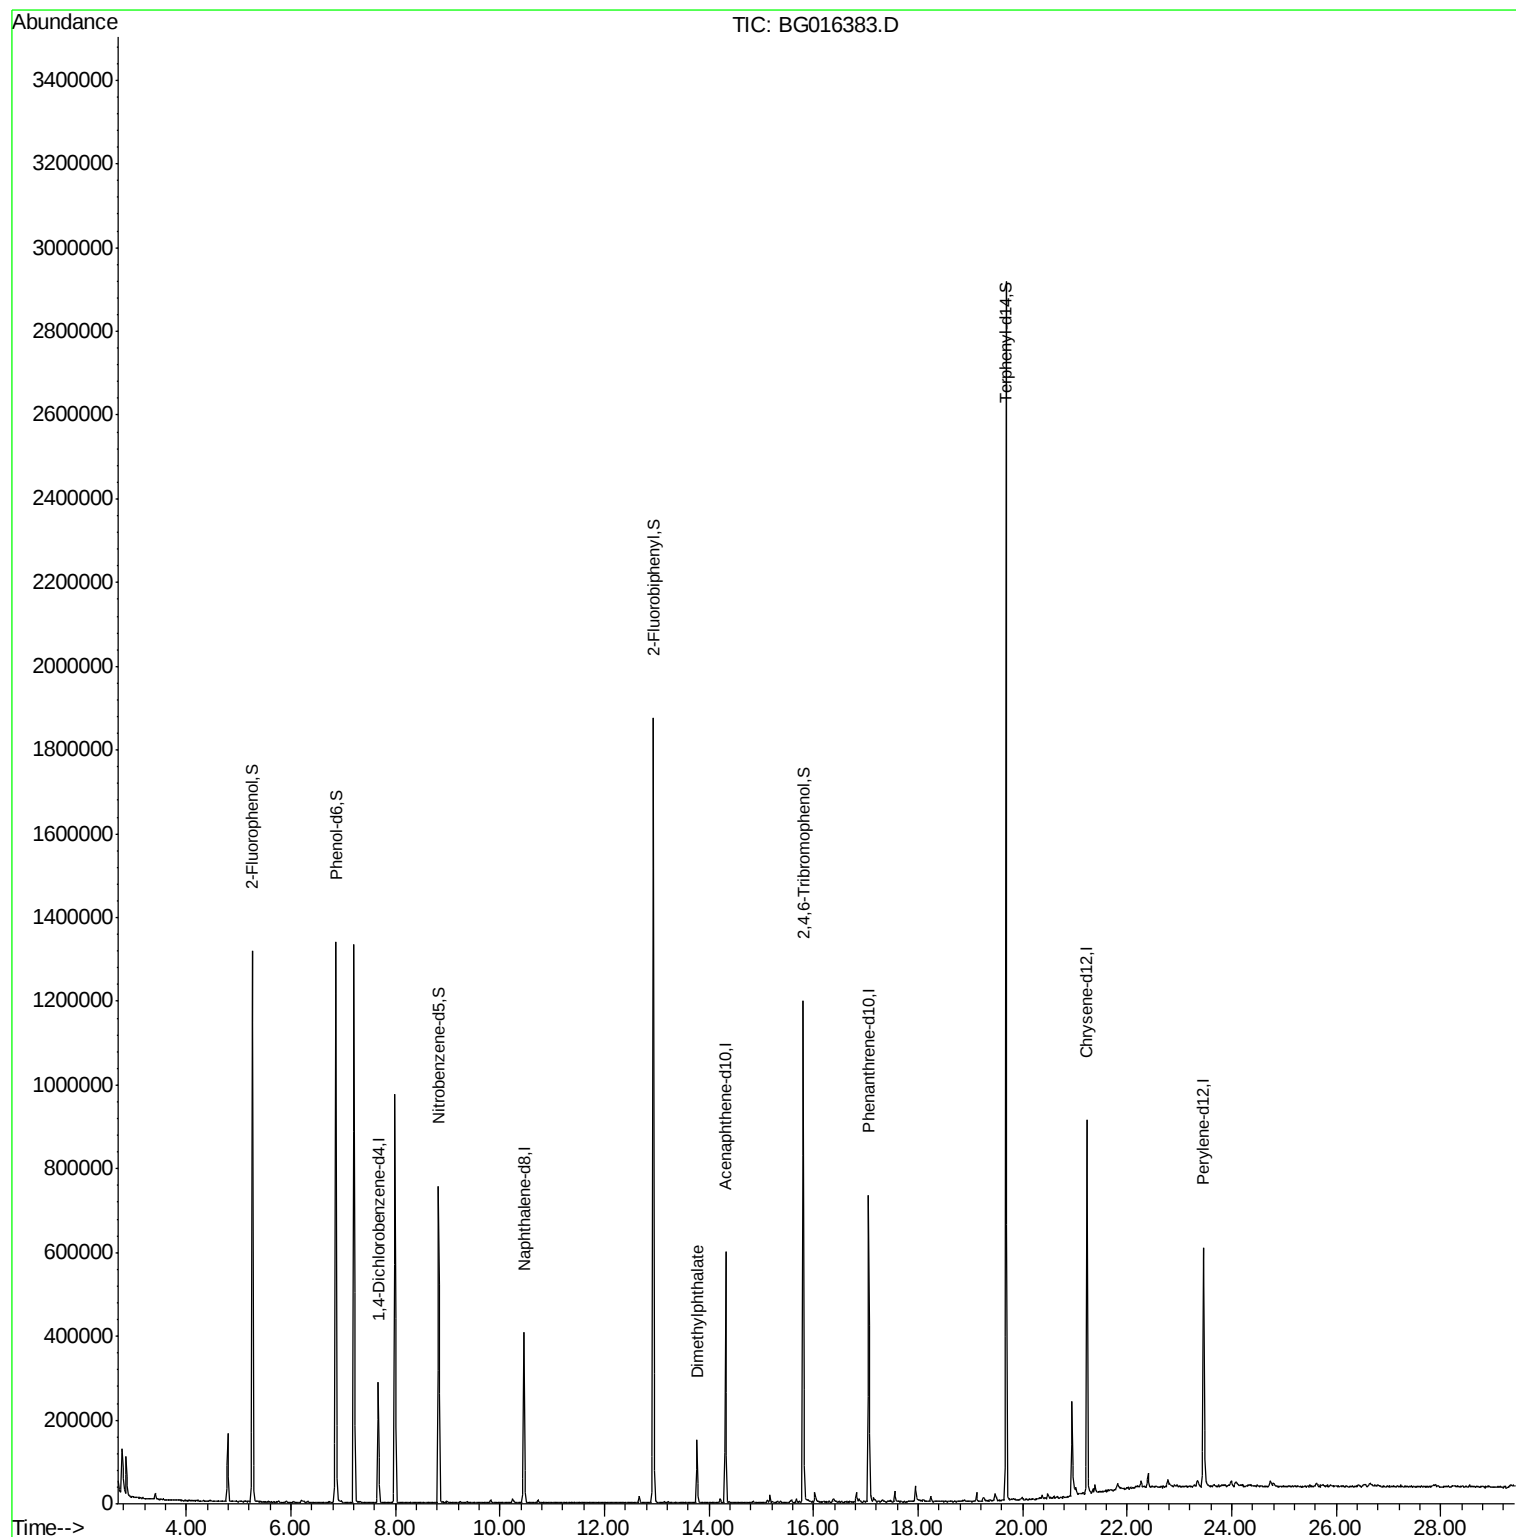



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.68 min Scan# 849

Delta R.T. 0.00 min

Lab File: BG016383.D

Acq: 14 Apr 2015 6:02

Instrument :

BNA_G

ClientSampleId :

FS-027


Tgt Ion:152 Resp: 80968

Ion Ratio Lower Upper

152 100

150 155.0 130.1 195.1



115 57.6 50.5 75.7

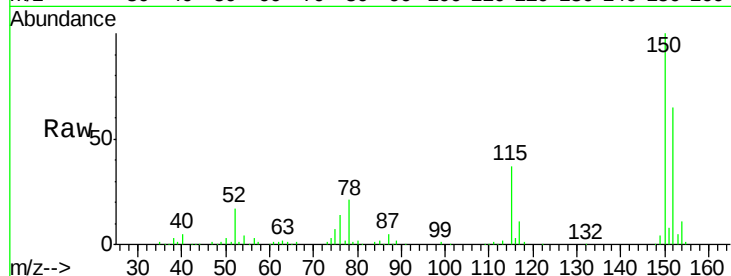

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

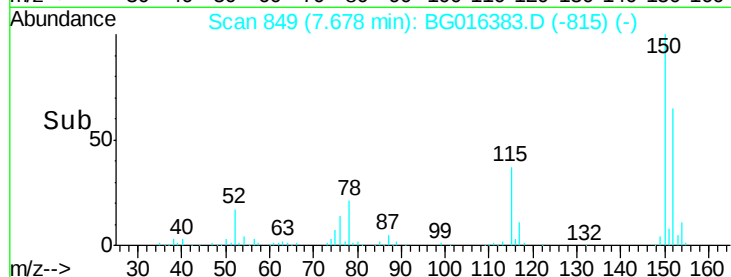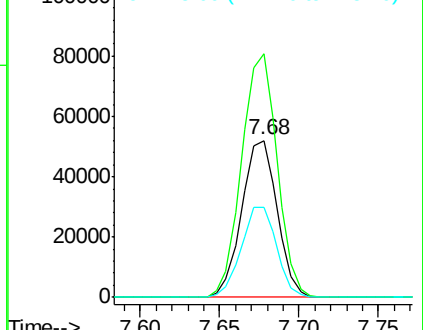

#5

2-Fluorophenol

Concen: 119.04 ng

RT: 5.26 min Scan# 438

Delta R.T. 0.00 min

Lab File: BG016383.D

Acq: 14 Apr 2015 6:02


Tgt Ion:112 Resp: 610735

Ion Ratio Lower Upper

112 100

64 54.4 44.5 66.7



63 25.3 21.4 32.0




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

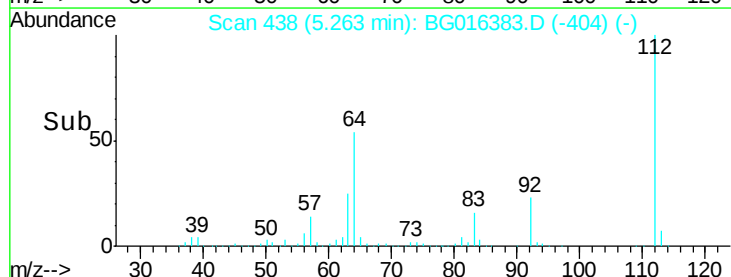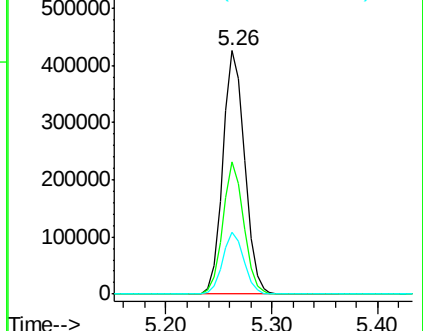

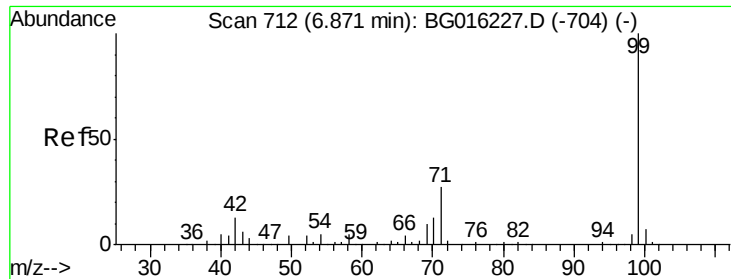

#7

Phenol-d6

Concen: 111.63 ng

RT: 6.86 min Scan# 710

Delta R.T. 0.00 min

Lab File: BG016383.D

Acq: 14 Apr 2015 6:02

Instrument :

BNA_G

ClientSampleId :

FS-027


Tgt Ion: 99 Resp: 859758

Ion Ratio Lower Upper




99 100

42 12.2 10.0 15.0

71 26.5 21.5 32.3



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

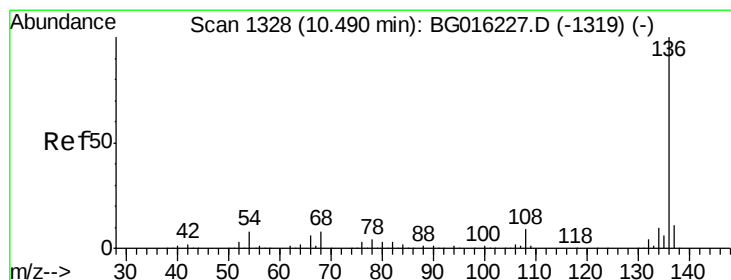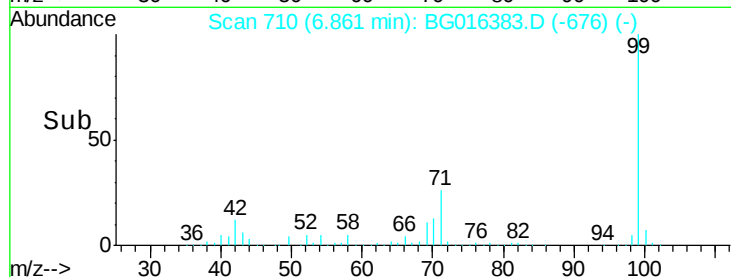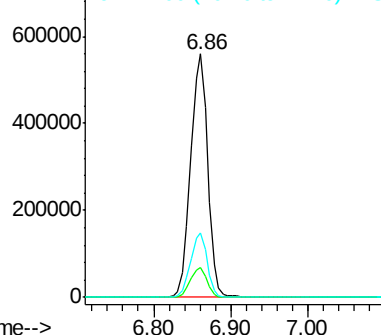

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.46 min Scan# 1323

Delta R.T. 0.00 min

Lab File: BG016383.D

Acq: 14 Apr 2015 6:02

Tgt Ion: 136 Resp: 349046


Ion Ratio Lower Upper

136 100



137 11.6 8.7 13.1

54 7.1 6.3 9.5

68 6.9 6.5 9.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

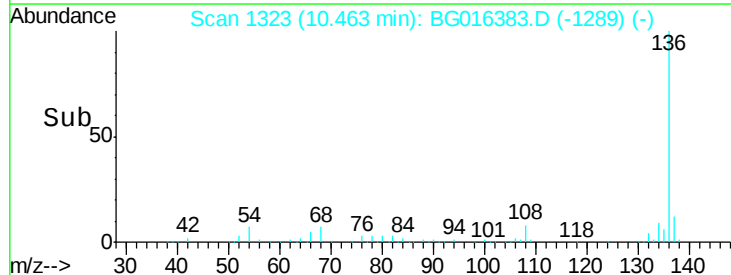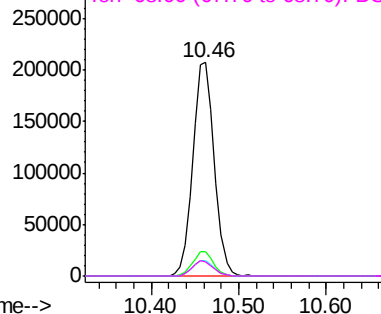







#23
 Nitrobenzene-d5
 Concen: 74.79 ng
 RT: 8.83 min Scan# 1045
 Delta R.T. -0.00 min
 Lab File: BG016383.D
 Acq: 14 Apr 2015 6:02

Instrument :
 BNA_G
 ClientSampleId :
 FS-027

Tgt Ion: 82 Resp: 450649
 Ion Ratio Lower Upper
 82 100
 128 50.4 37.8 56.8
 54 40.0 32.6 49.0

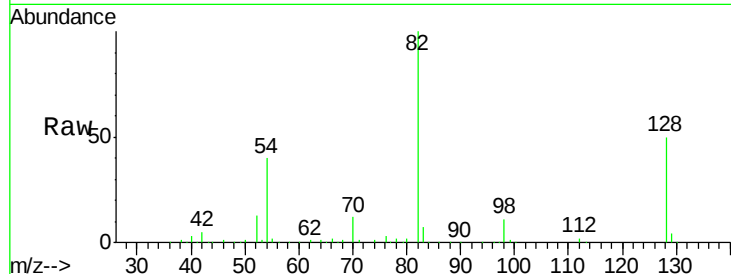


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

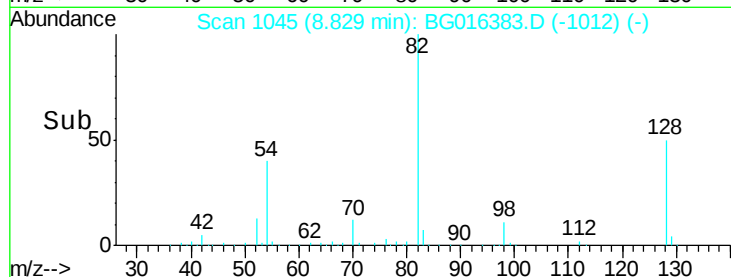
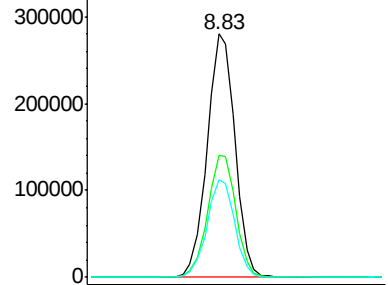



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.32 min Scan# 1979
 Delta R.T. 0.00 min
 Lab File: BG016383.D
 Acq: 14 Apr 2015 6:02

Tgt Ion: 164 Resp: 189445
 Ion Ratio Lower Upper
 164 100
 162 97.5 77.3 115.9
 160 44.5 36.7 55.1



Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC



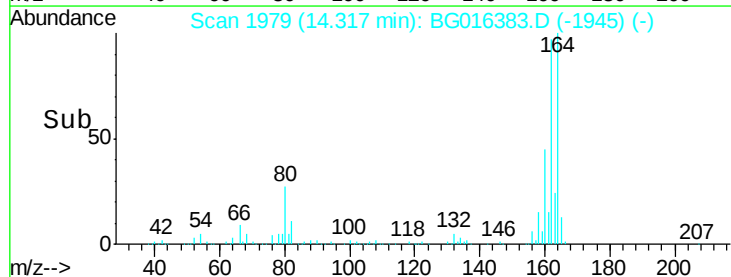
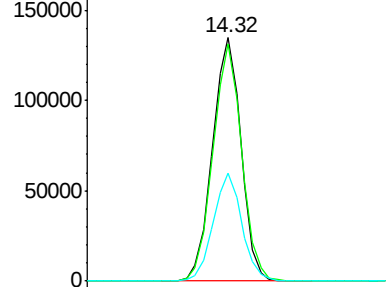


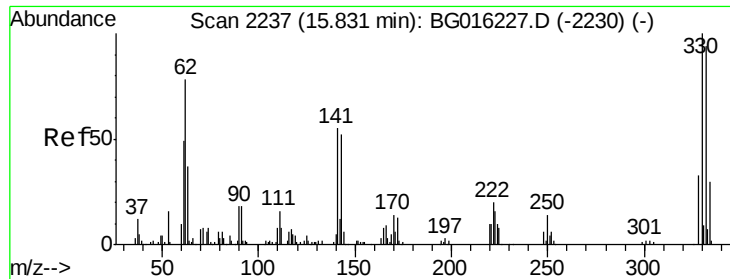

#41
 2,4,6-Tribromophenol
 Concen: 127.50 ng
 RT: 15.81 min Scan# 2233
 Delta R.T. 0.00 min
 Lab File: BG016383.D
 Acq: 14 Apr 2015 6:02




Instrument :
 BNA_G
 ClientSampleId :
 FS-027

Tgt Ion: 330 Resp: 163351
 Ion Ratio Lower Upper
 330 100
 332 95.2 75.8 113.6
 141 55.5 46.6 69.8

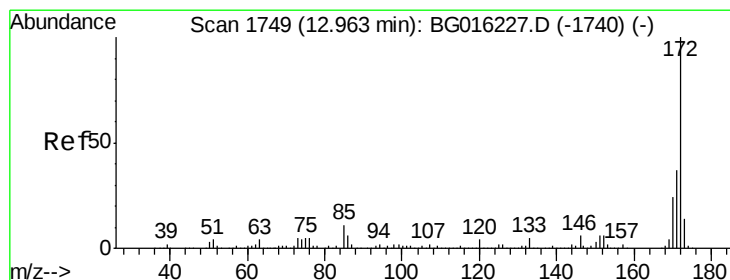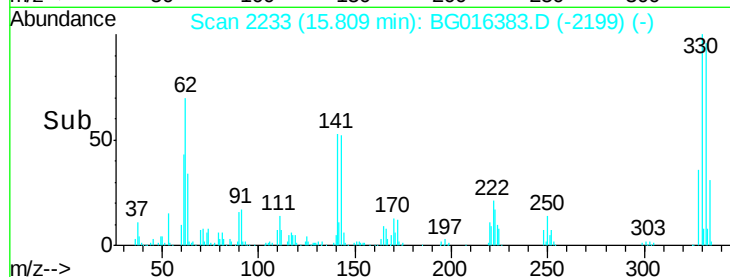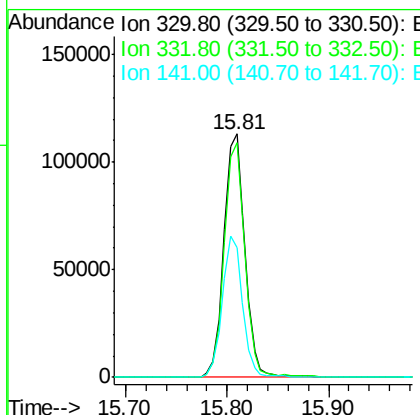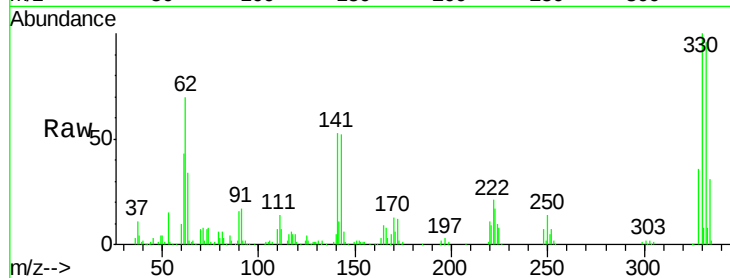

#44
 2-Fluorobiphenyl
 Concen: 79.92 ng
 RT: 12.94 min Scan# 1744
 Delta R.T. -0.00 min
 Lab File: BG016383.D
 Acq: 14 Apr 2015 6:02

Tgt Ion: 172 Resp: 889269
 Ion Ratio Lower Upper
 172 100
 171 37.6 29.6 44.4
 170 24.7 19.4 29.2

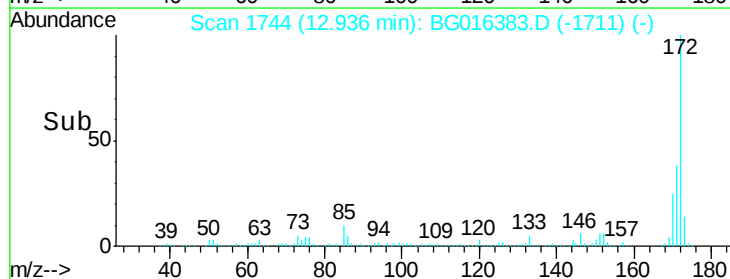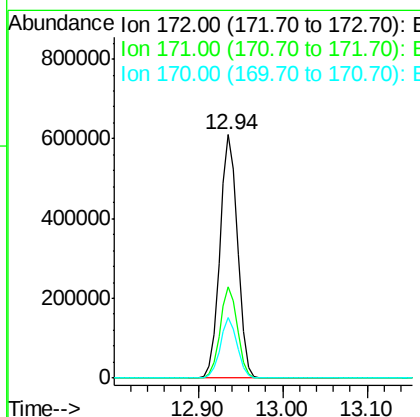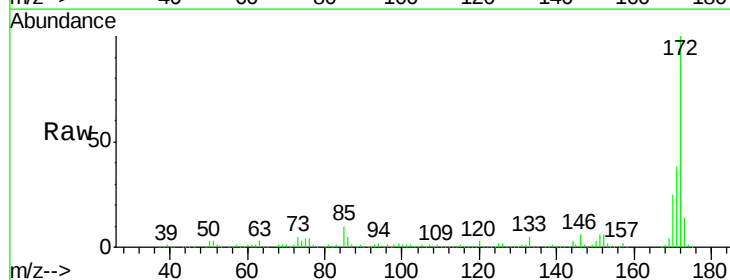







#49
Dimethylphthalate
Concen: 6.88 ng
RT: 13.78 min Scan# 1887
Delta R.T. -0.00 min
Lab File: BG016383.D
Acq: 14 Apr 2015 6:02

Instrument :
BNA_G
ClientSampleId :
FS-027

Tgt Ion:163 Resp: 95576
Ion Ratio Lower Upper
163 100
194 6.9 5.0 7.4
164 9.4 8.2 12.4




Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

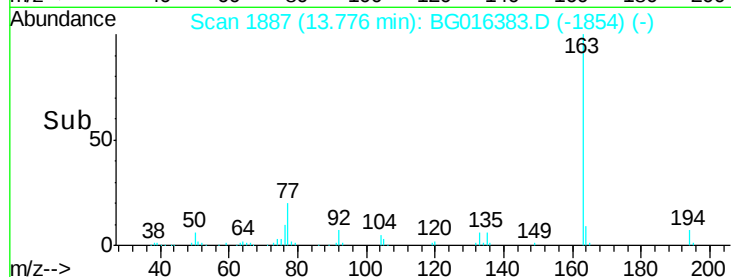
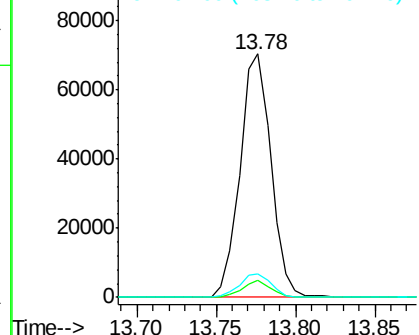



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.05 min Scan# 2445
Delta R.T. -0.00 min
Lab File: BG016383.D
Acq: 14 Apr 2015 6:02

Tgt Ion:188 Resp: 391920
Ion Ratio Lower Upper
188 100
94 14.7 12.2 18.4
80 15.2 12.8 19.2



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BG0
Ion 80.00 (79.70 to 80.70): BG0

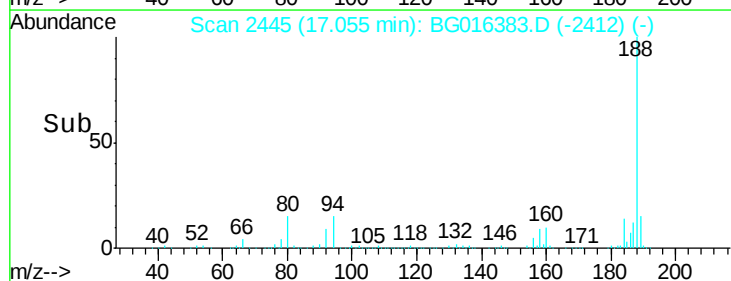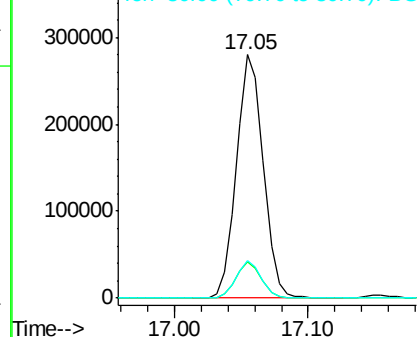

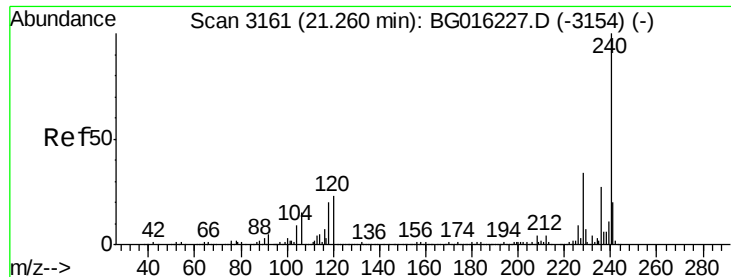

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.23 min Scan# 3156

Delta R.T. -0.00 min

Lab File: BG016383.D

Acq: 14 Apr 2015 6:02

Instrument :

BNA_G

ClientSampleId :

FS-027


Tgt Ion:240 Resp: 361112

Ion Ratio Lower Upper

240 100

120 21.9 18.6 28.0




236 25.7 21.7 32.5



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

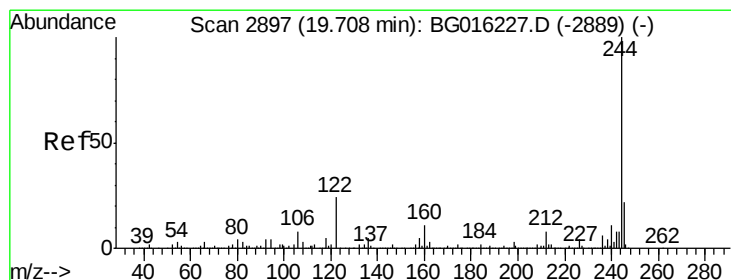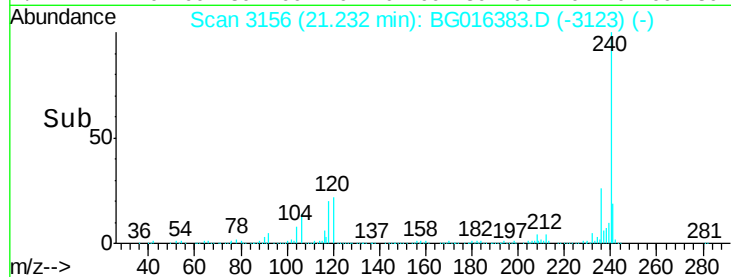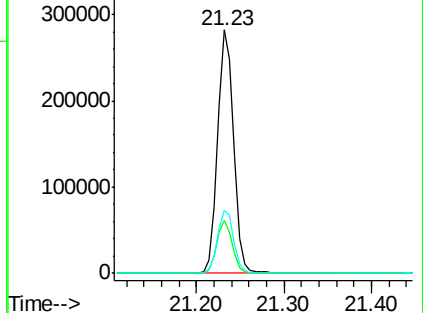

#78

Terphenyl-d14

Concen: 67.34 ng

RT: 19.69 min Scan# 2893

Delta R.T. 0.00 min

Lab File: BG016383.D

Acq: 14 Apr 2015 6:02


Tgt Ion:244 Resp: 1039015

Ion Ratio Lower Upper

244 100

212 8.0 6.6 9.8



122 22.3 19.1 28.7




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

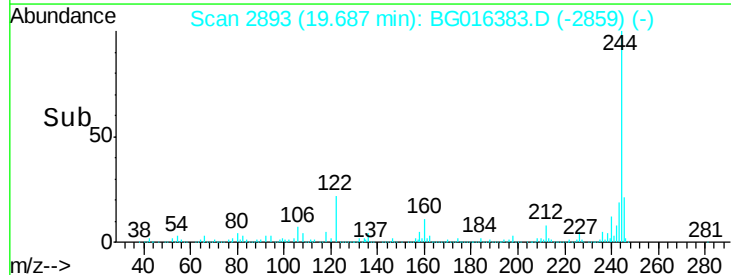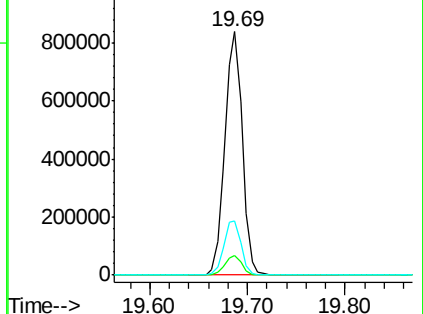

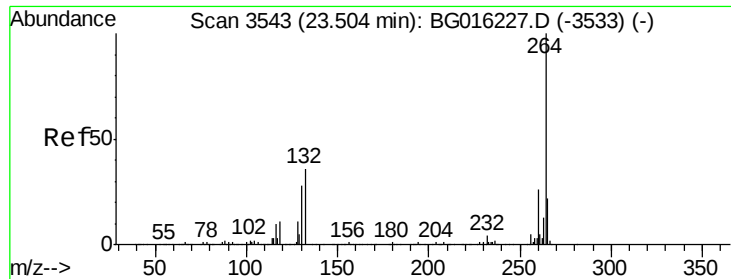

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.47 min Scan# 3537

Delta R.T. 0.00 min

Lab File: BG016383.D

Acq: 14 Apr 2015 6:02

Instrument :

BNA_G

ClientSampleId :

FS-027


Tgt Ion: 264 Resp: 339803

Ion Ratio Lower Upper

264 100

260 24.8 20.4 30.6

265 21.2 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

