

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041316\
 Data File : BG021643.D
 Acq On : 14 Apr 2016 6:55
 Operator : UM/SJ
 Sample : H2418-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GMW-9

Quant Time: Apr 14 07:36:33 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 15:48:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.21	152	30121	20.00	ng	0.00
21) Naphthalene-d8	11.03	136	140459	20.00	ng	0.00
38) Acenaphthene-d10	14.82	164	90662	20.00	ng	0.00
63) Phenanthrene-d10	17.56	188	218882	20.00	ng	0.00
75) Chrysene-d12	21.83	240	251961	20.00	ng	0.00
86) Perylene-d12	25.15	264	243646	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.76	112	178270	98.56	ng	0.00
7) Phenol-d6	7.36	99	185718	68.74	ng	0.00
23) Nitrobenzene-d5	9.38	82	277832	101.67	ng	0.00
41) 2,4,6-Tribromophenol	16.30	330	162608	166.42	ng	0.00
44) 2-Fluorobiphenyl	13.46	172	629539	101.74	ng	0.00
78) Terphenyl-d14	20.15	244	830077	82.20	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.64	88	3046	3.78	ng	# 64
18) Hexachloroethane	9.33	117	2575	2.87	ng	# 1
32) Benzoic acid	10.23	122	741	4.86	ng	86
36) 4-Chloro-3-methylphenol	12.34	107	7207	2.65	ng	# 22
49) Dimethylphthalate	14.27	163	16002	2.04	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041316\
Data File : BG021643.D
Acq On : 14 Apr 2016 6:55
Operator : UM/SJ
Sample : H2418-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GMW-9

Quant Time: Apr 14 07:36:33 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

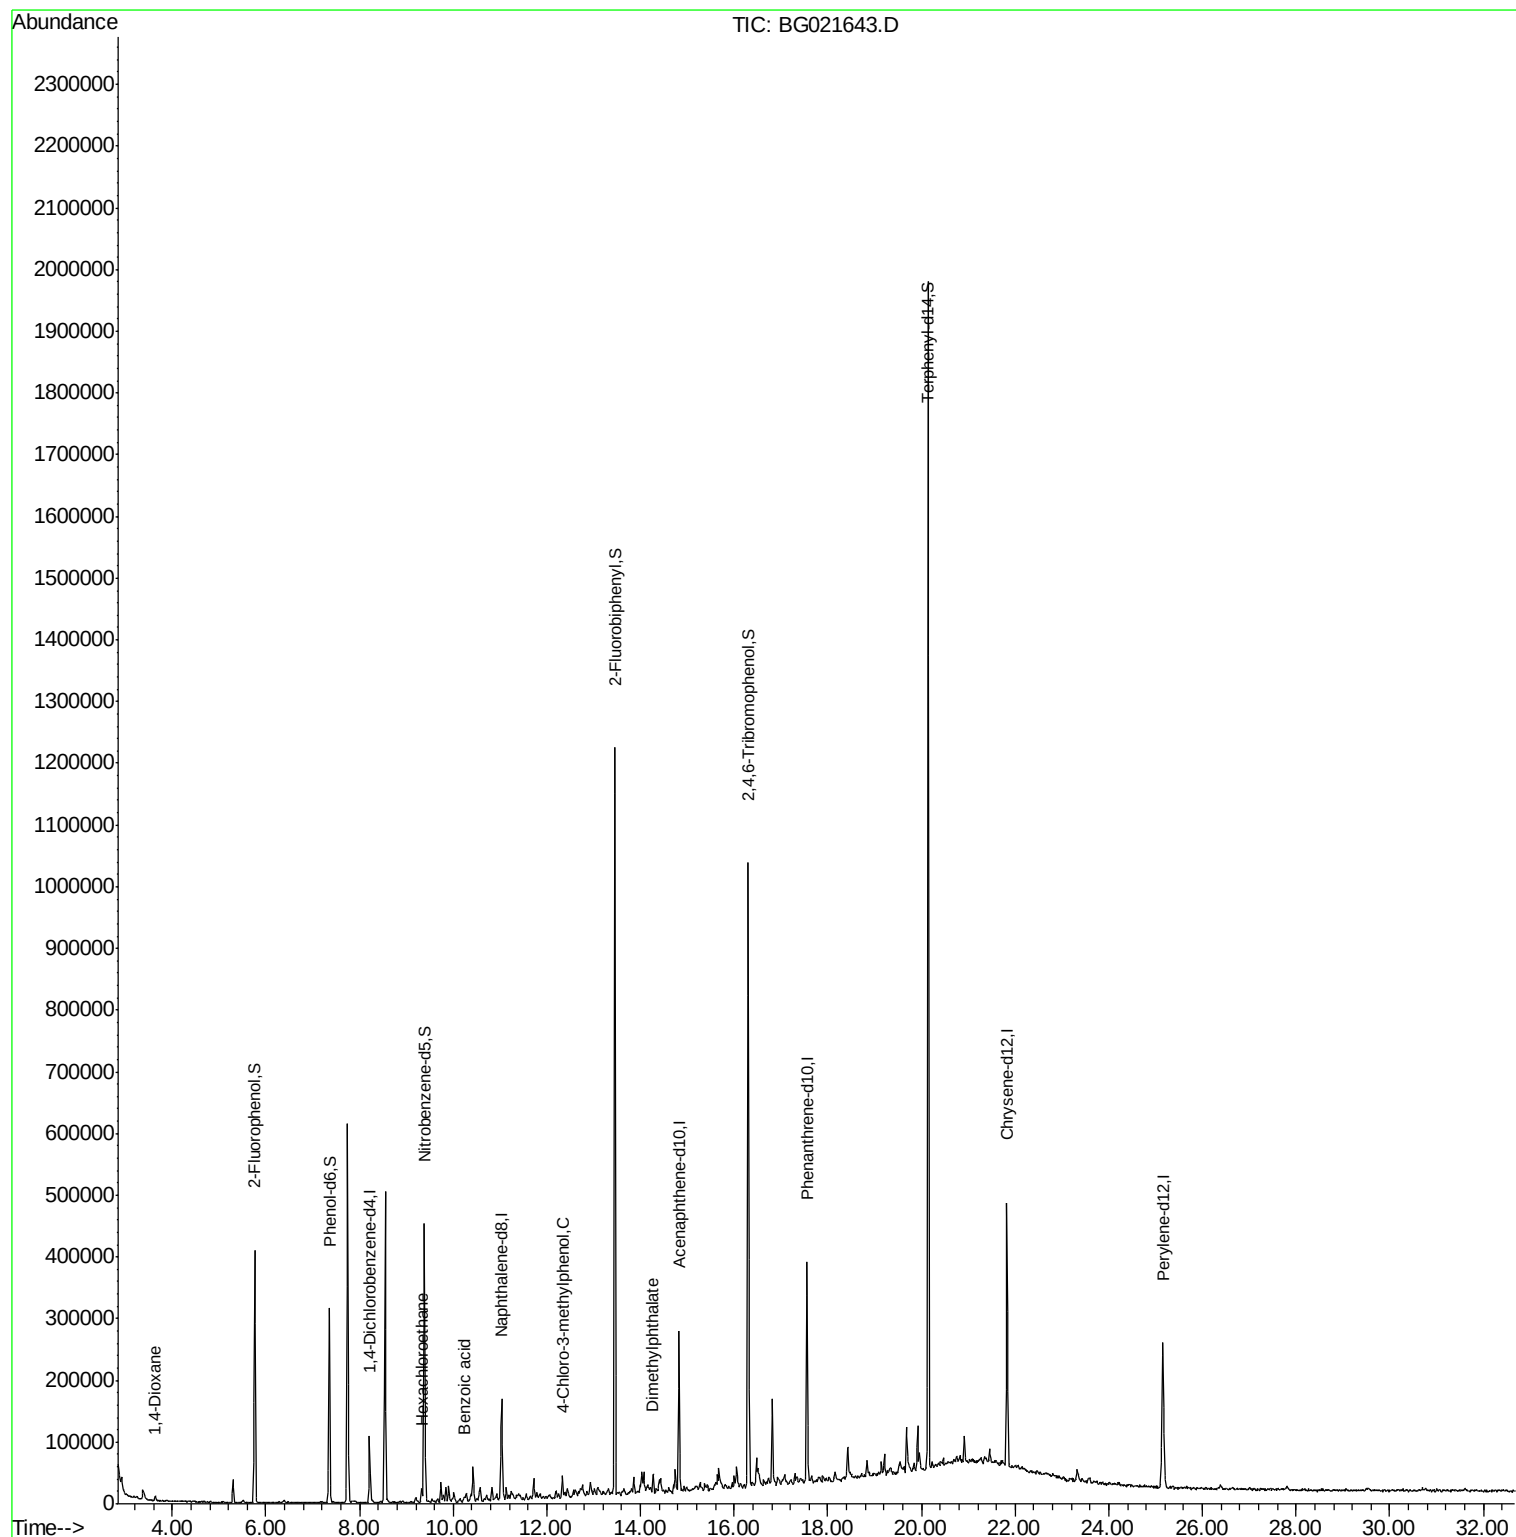

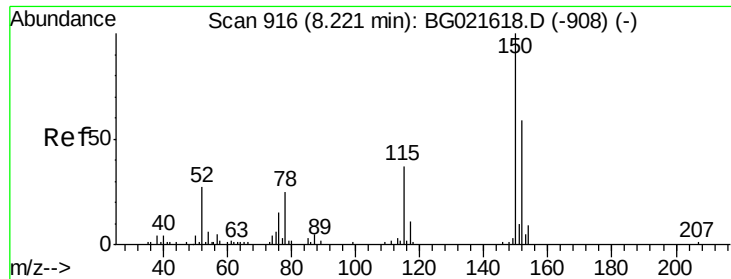

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.21 min Scan# 915

Delta R.T. -0.01 min

Lab File: BG021643.D

Acq: 14 Apr 2016 6:55

Instrument :

BNA_G

ClientSampleId :

GMW-9


Tgt Ion:152 Resp: 30121

Ion Ratio Lower Upper

152 100

150 170.0 130.1 195.1




115 64.5 62.2 93.2



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

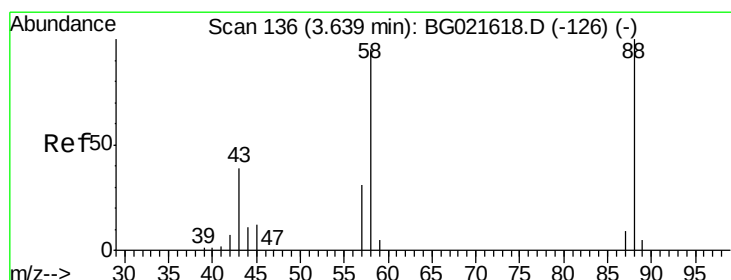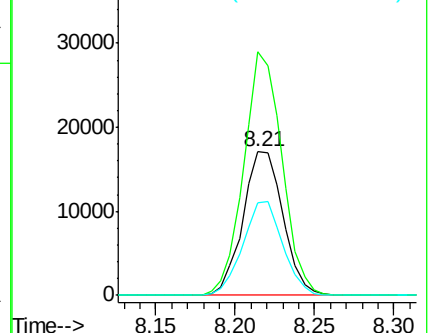

#2

1,4-Dioxane

Concen: 3.78 ng

RT: 3.64 min Scan# 136

Delta R.T. -0.00 min

Lab File: BG021643.D

Acq: 14 Apr 2016 6:55


Tgt Ion: 88 Resp: 3046

Ion Ratio Lower Upper

88 100

58 100.4 61.8 92.8#



43 67.4 27.3 40.9#




Abundance Ion 88.00 (87.70 to 88.70): BGC

Ion 58.00 (57.70 to 58.70): BGC

Ion 43.00 (42.70 to 43.70): BGC

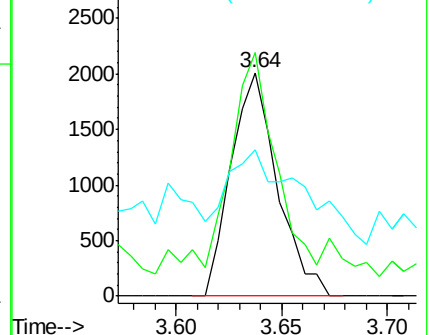



#5

2-Fluorophenol

Concen: 98.56 ng

RT: 5.76 min Scan# 498

Delta R.T. 0.01 min

Lab File: BG021643.D

Acq: 14 Apr 2016 6:55

Instrument :

BNA_G

ClientSampleID :

GMW-9


Tgt Ion: 112 Resp: 178270

Ion Ratio Lower Upper

112 100

64 67.7 51.1 76.7




63 34.3 24.6 37.0



Abundance Ion 112.00 (111.70 to 112.70): BGC

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

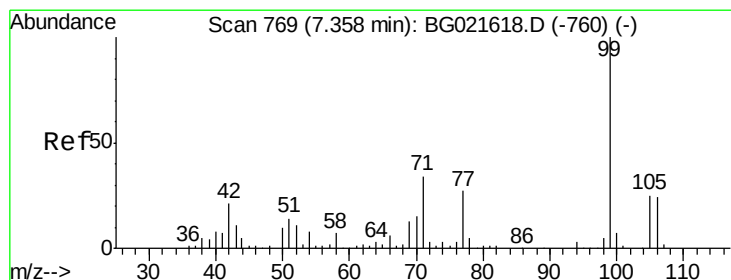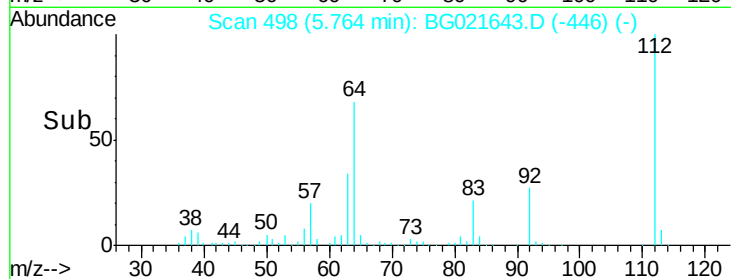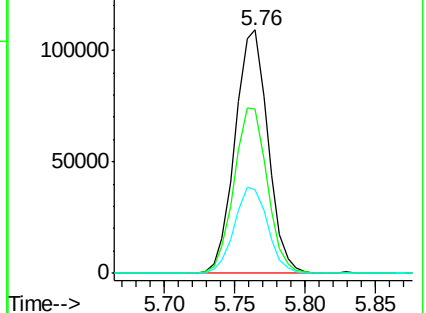

#7

Phenol-d6

Concen: 68.74 ng

RT: 7.36 min Scan# 769

Delta R.T. -0.00 min

Lab File: BG021643.D

Acq: 14 Apr 2016 6:55


Tgt Ion: 99 Resp: 185718

Ion Ratio Lower Upper

99 100

42 20.0 16.4 24.6



71 34.0 25.0 37.4




Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC




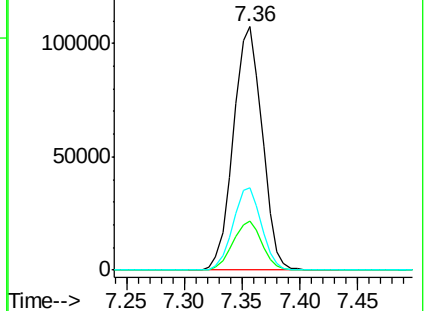




#18
Hexachloroethane
Concen: 2.87 ng
RT: 9.33 min Scan# 1105
Delta R.T. 0.02 min
Lab File: BG021643.D
Acq: 14 Apr 2016 6:55




Instrument :
BNA_G
ClientSampleId :
GMW-9


Tgt Ion:117 Resp: 2575
Ion Ratio Lower Upper
117 100
119 501.0 63.9 95.9#
201 0.0 61.2 91.8#

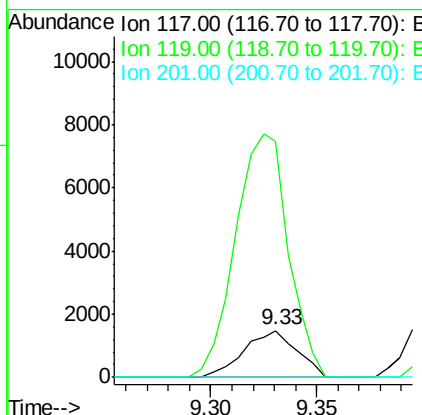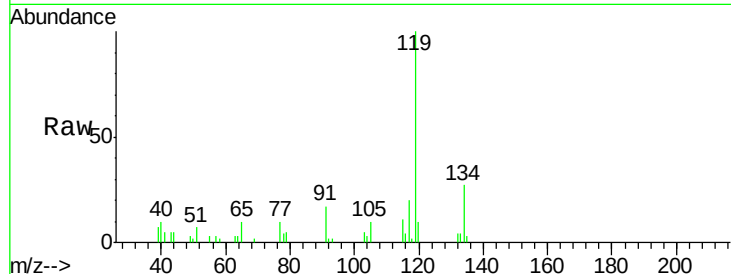

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.03 min Scan# 1395
Delta R.T. -0.00 min
Lab File: BG021643.D
Acq: 14 Apr 2016 6:55

Tgt Ion:136 Resp: 140459
Ion Ratio Lower Upper
136 100
137 10.0 9.0 13.4
54 11.4 9.6 14.4
68 7.0 6.4 9.6



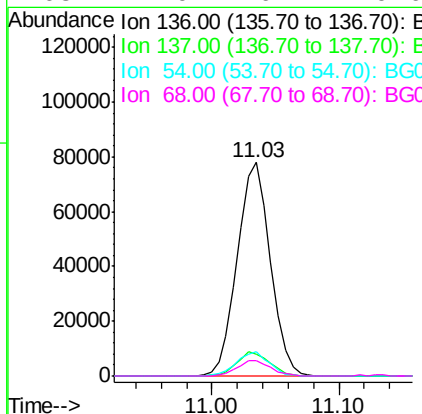
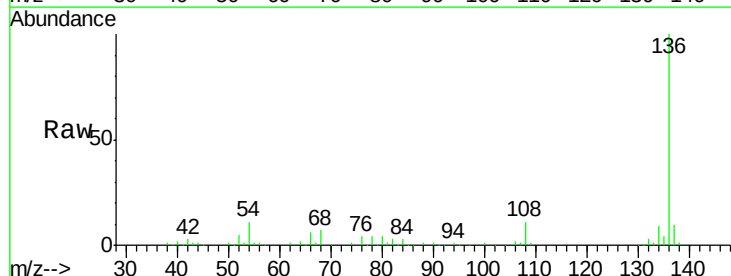


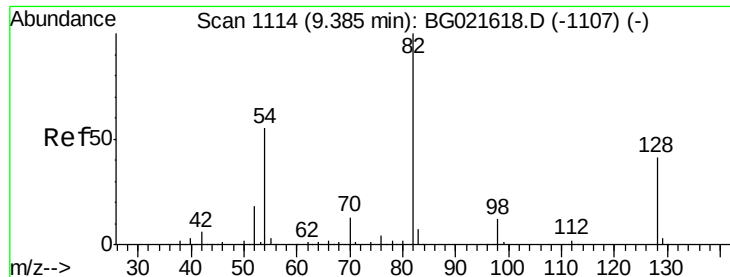

#23
 Nitrobenzene-d5
 Concen: 101.67 ng
 RT: 9.38 min Scan# 1114
 Delta R.T. -0.00 min
 Lab File: BG021643.D
 Acq: 14 Apr 2016 6:55




Instrument :
 BNA_G
 ClientSampleId :
 GMW-9


Tgt Ion: 82 Resp: 277832
 Ion Ratio Lower Upper
 82 100
 128 41.7 33.4 50.0
 54 56.8 46.1 69.1

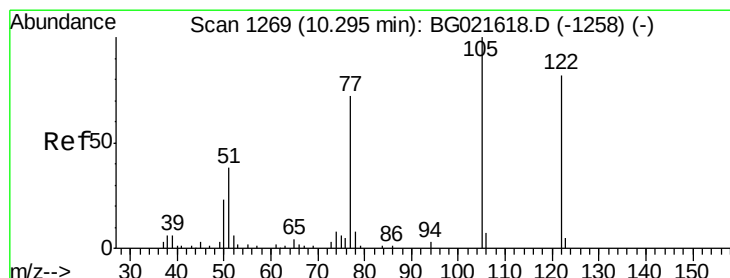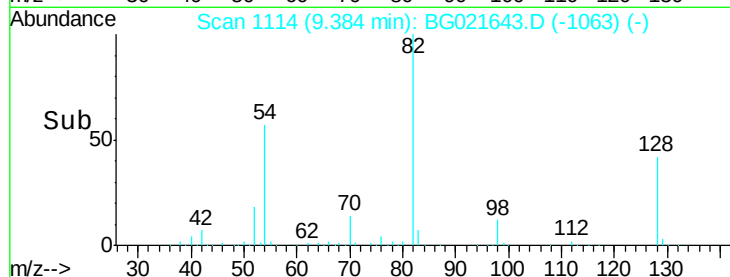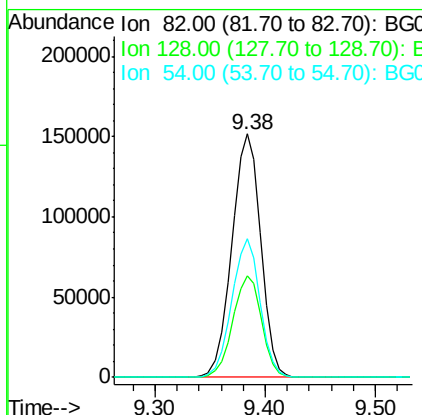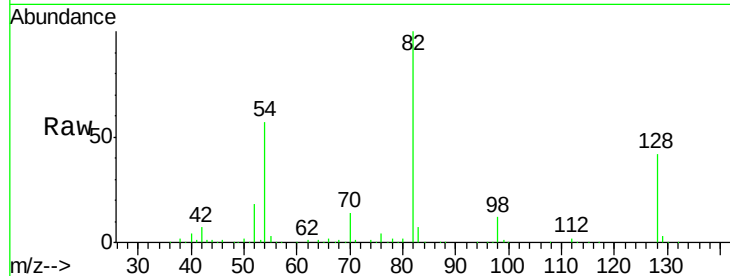

#32
 Benzoic acid
 Concen: 4.86 ng
 RT: 10.23 min Scan# 1258
 Delta R.T. -0.07 min
 Lab File: BG021643.D
 Acq: 14 Apr 2016 6:55

Tgt Ion: 122 Resp: 741
 Ion Ratio Lower Upper
 122 100
 105 138.0 104.5 144.5
 77 82.2 79.9 119.9


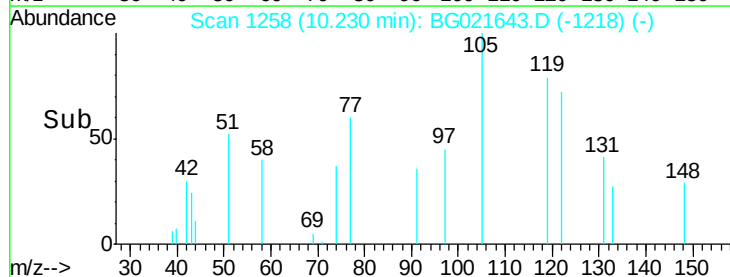
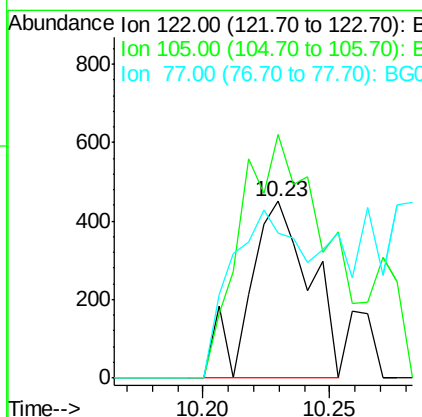
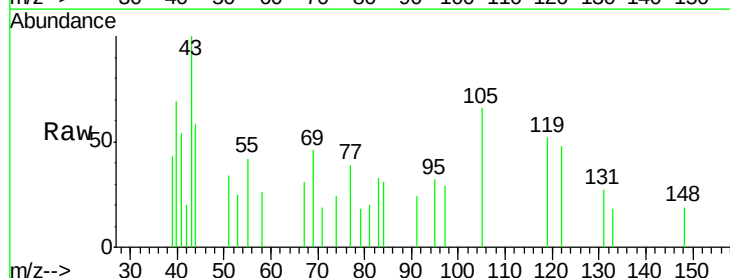


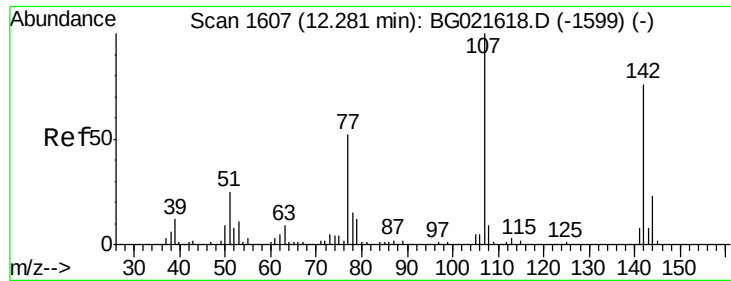

#36
 4-Chloro-3-methylphenol
 Concen: 2.65 ng
 RT: 12.34 min Scan# 1617
 Delta R.T. 0.06 min
 Lab File: BG021643.D
 Acq: 14 Apr 2016 6:55




Instrument :
 BNA_G
 ClientSampleId :
 GMW-9


Tgt Ion:107 Resp: 7207
 Ion Ratio Lower Upper
 107 100
 144 0.0 19.2 28.8#
 142 0.0 59.1 88.7#

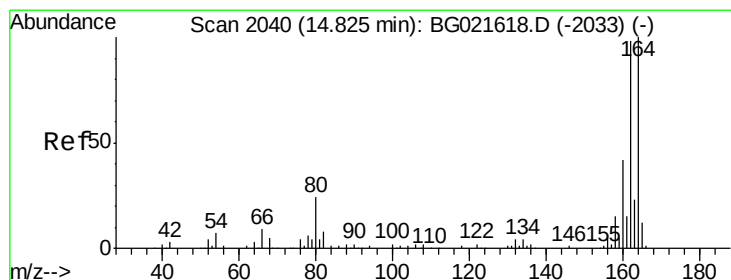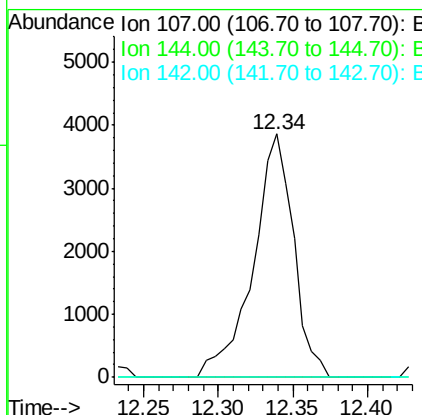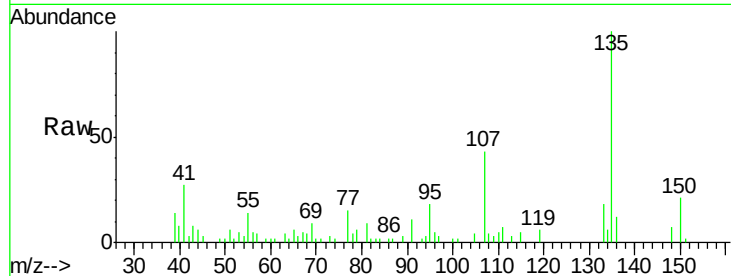

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.82 min Scan# 2040
 Delta R.T. -0.00 min
 Lab File: BG021643.D
 Acq: 14 Apr 2016 6:55

Tgt Ion:164 Resp: 90662
 Ion Ratio Lower Upper
 164 100
 162 101.3 78.0 117.0
 160 49.1 32.9 49.3

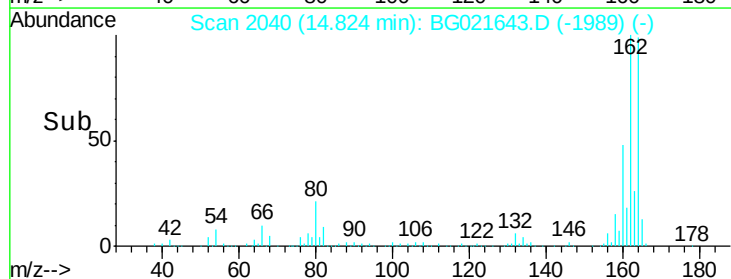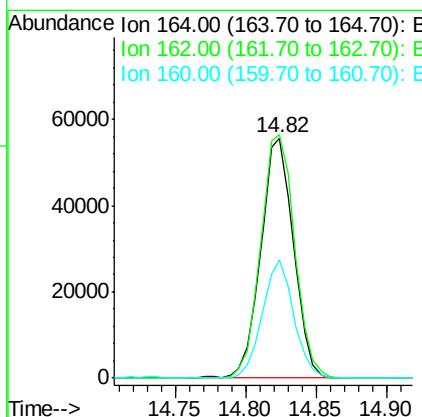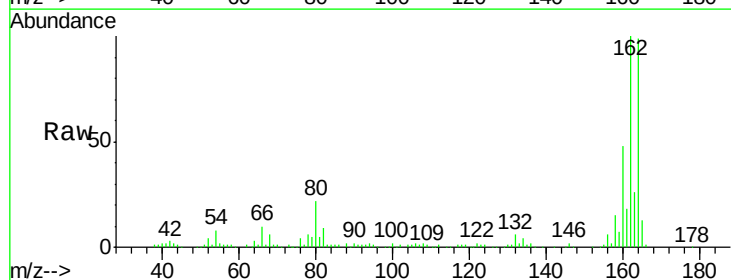


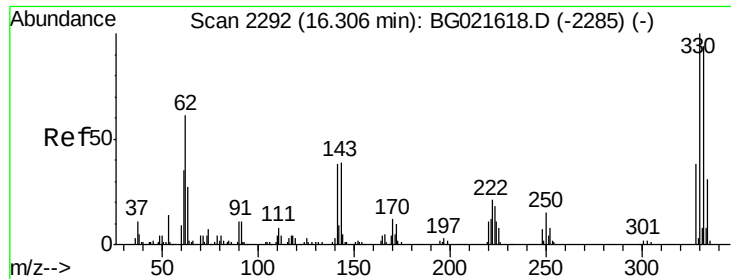




#41
 2,4,6-Tribromophenol
 Concen: 166.42 ng
 RT: 16.30 min Scan# 2291
 Delta R.T. -0.01 min
 Lab File: BG021643.D
 Acq: 14 Apr 2016 6:55

Instrument :
 BNA_G
 ClientSampleId :
 GMW-9

Tgt Ion:330 Resp: 162608
 Ion Ratio Lower Upper
 330 100
 332 97.4 78.0 117.0
 141 41.7 33.8 50.8




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


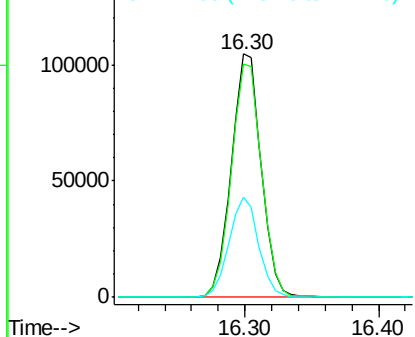



#44
 2-Fluorobiphenyl
 Concen: 101.74 ng
 RT: 13.46 min Scan# 1807
 Delta R.T. -0.00 min
 Lab File: BG021643.D
 Acq: 14 Apr 2016 6:55

Tgt Ion:172 Resp: 629539
 Ion Ratio Lower Upper
 172 100
 171 37.2 27.8 41.6
 170 25.5 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

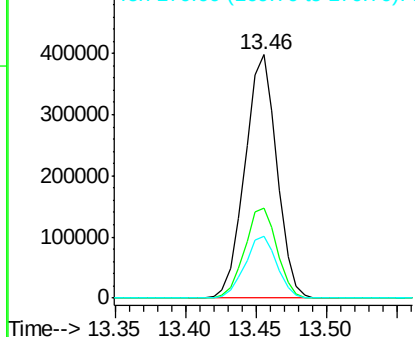

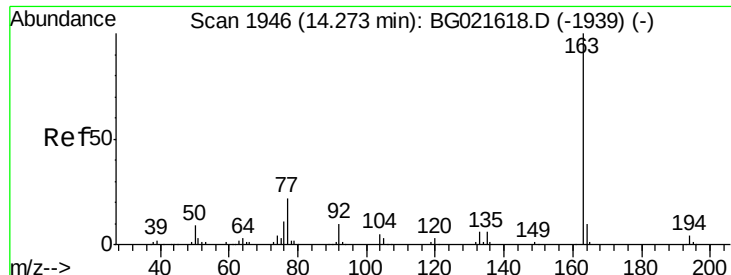

#49

Dimethylphthalate

Concen: 2.04 ng

RT: 14.27 min Scan# 1945

Delta R.T. -0.01 min

Lab File: BG021643.D

Acq: 14 Apr 2016 6:55

Instrument :

BNA_G

ClientSampleId :

GMW-9


Tgt Ion:163 Resp: 16002

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6




164 10.2 8.1 12.1



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

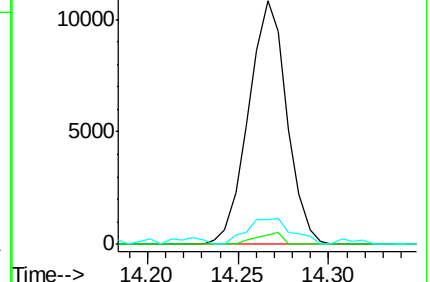

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.56 min Scan# 2505

Delta R.T. -0.01 min

Lab File: BG021643.D

Acq: 14 Apr 2016 6:55


Tgt Ion:188 Resp: 218882

Ion Ratio Lower Upper

188 100

94 10.6 7.5 11.3



80 11.5 8.6 13.0




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG0

Ion 80.00 (79.70 to 80.70): BG0



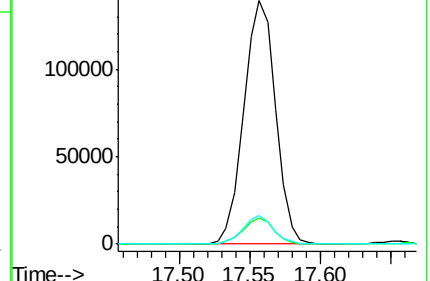



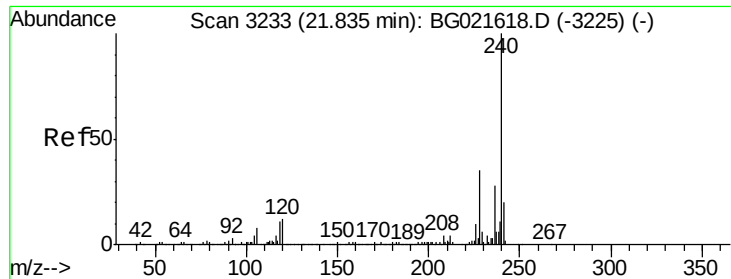

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.83 min Scan# 3232
Delta R.T. -0.01 min
Lab File: BG021643.D
Acq: 14 Apr 2016 6:55




Instrument :
BNA_G
ClientSampleId :
GMW-9


Tgt Ion:240 Resp: 251961
Ion Ratio Lower Upper
240 100
120 10.9 8.4 12.6
236 26.7 19.6 29.4

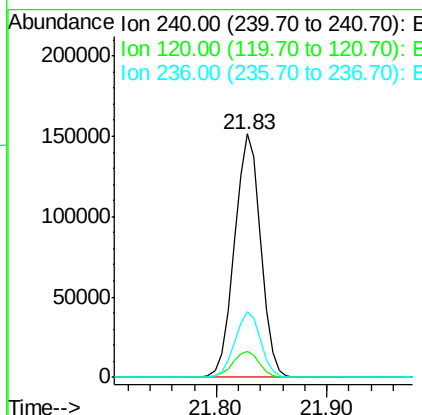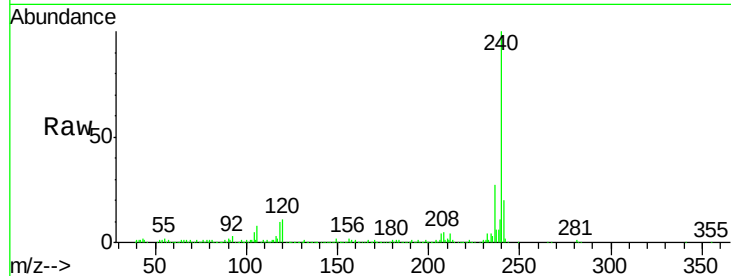

#78
Terphenyl-d14
Concen: 82.20 ng
RT: 20.15 min Scan# 2946
Delta R.T. -0.00 min
Lab File: BG021643.D
Acq: 14 Apr 2016 6:55

Tgt Ion:244 Resp: 830077
Ion Ratio Lower Upper
244 100
212 8.0 6.5 9.7
122 10.7 8.6 12.8

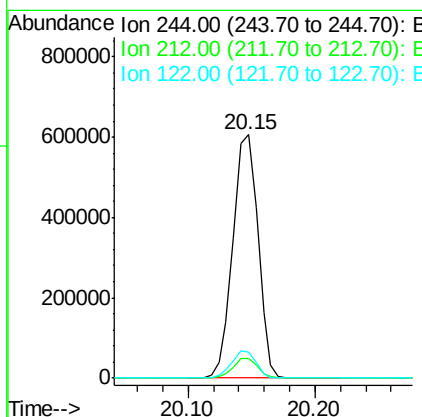

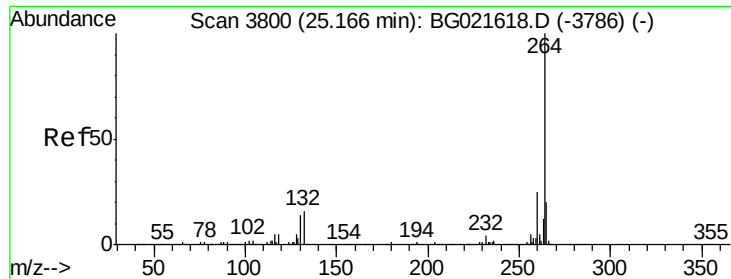

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.15 min Scan# 3798
Delta R.T. -0.01 min
Lab File: BG021643.D
Acq: 14 Apr 2016 6:55

Instrument :
BNA_G
ClientSampleId :
GMW-9

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.9	20.2	30.4
265	23.2	17.8	26.8

