
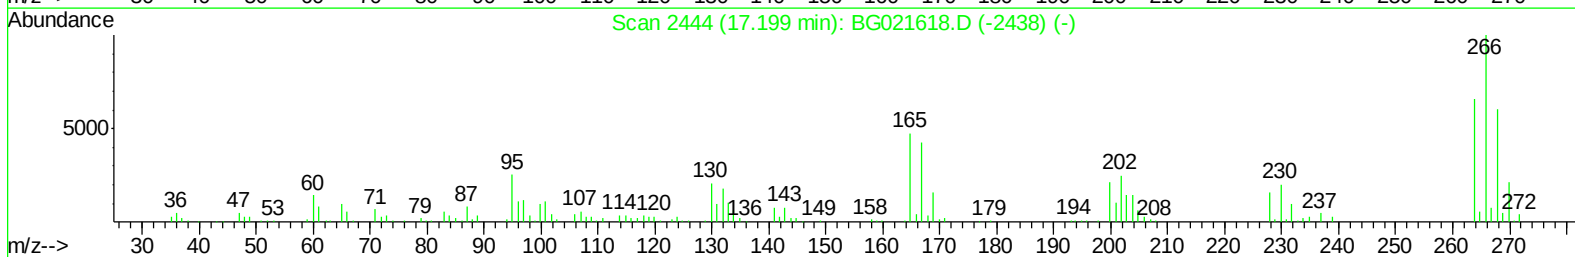
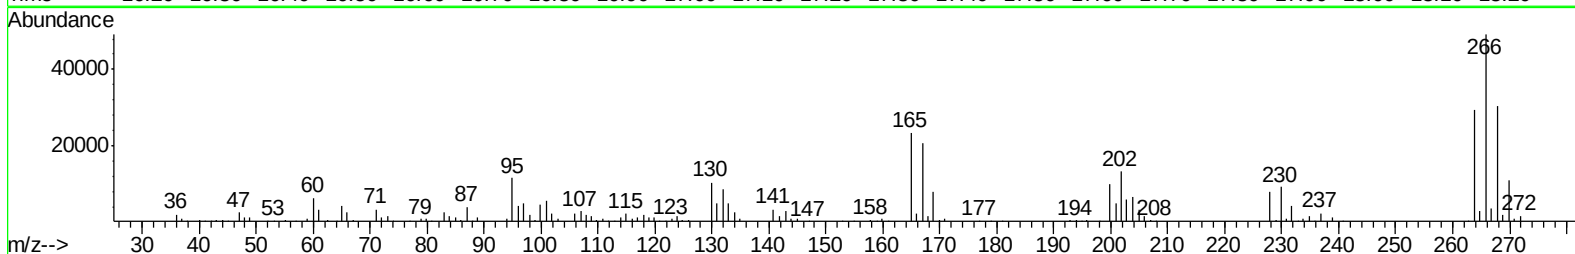


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041316\
Data File : BG021614.D
Acq On : 13 Apr 2016 10:17
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 04:39:03 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

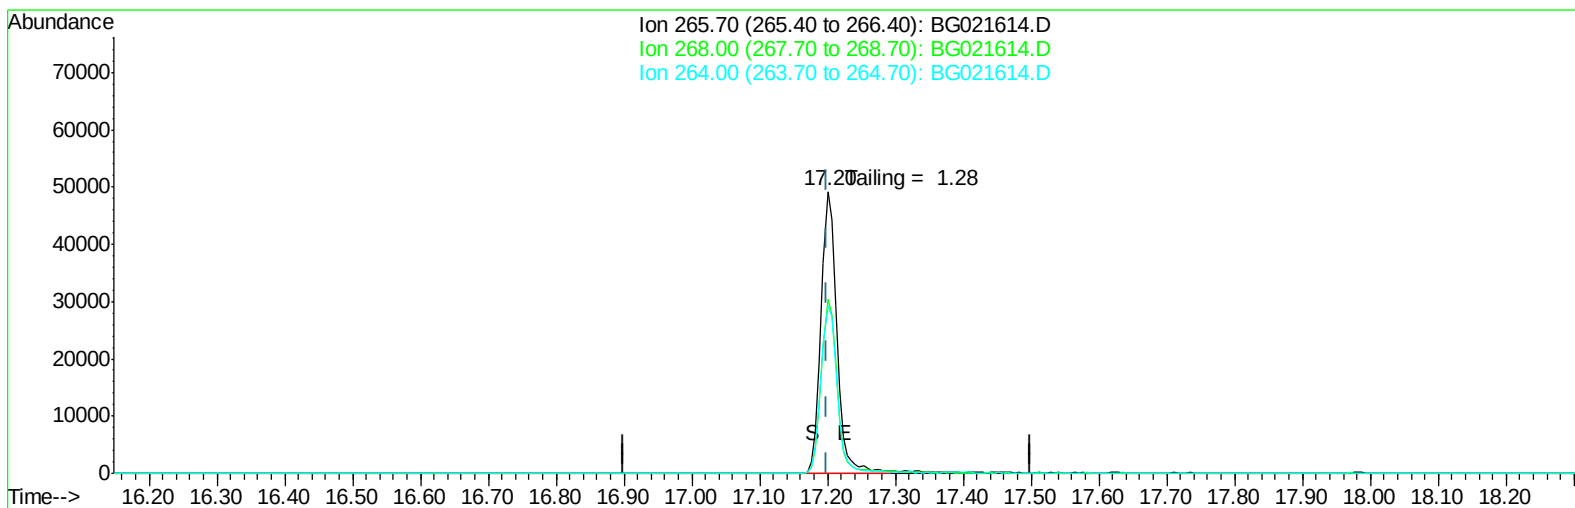

TIC: BG021614.D

(69) Pentachlorophenol (C)




17.200min (+0.001) 214381.90ng

response 78904

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	61.86
264.00	67.20	59.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041316\
Data File : BG021614.D
Acq On : 13 Apr 2016 10:17
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 04:39:03 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

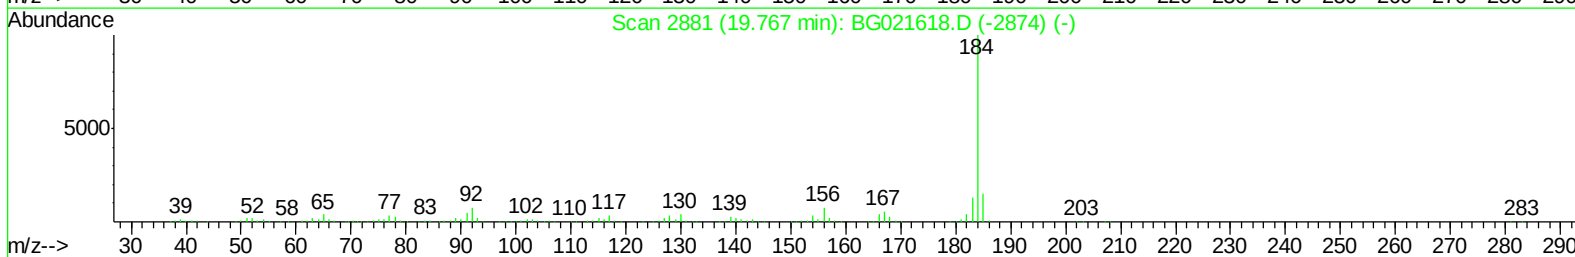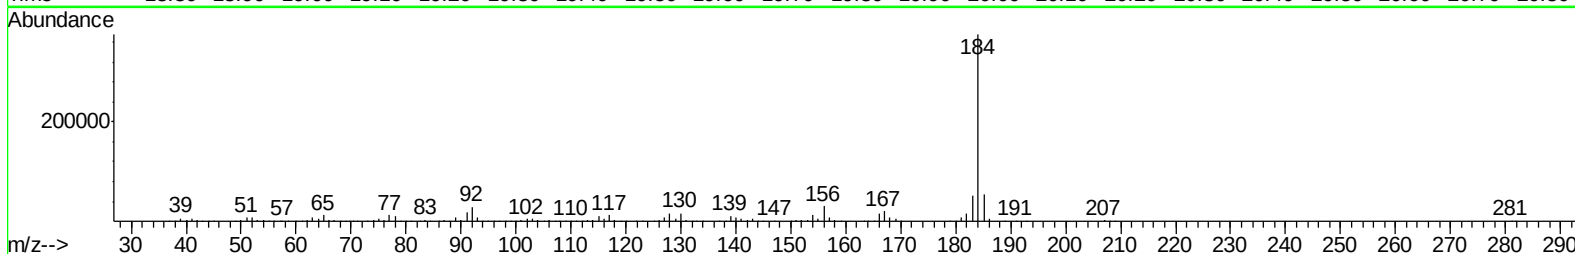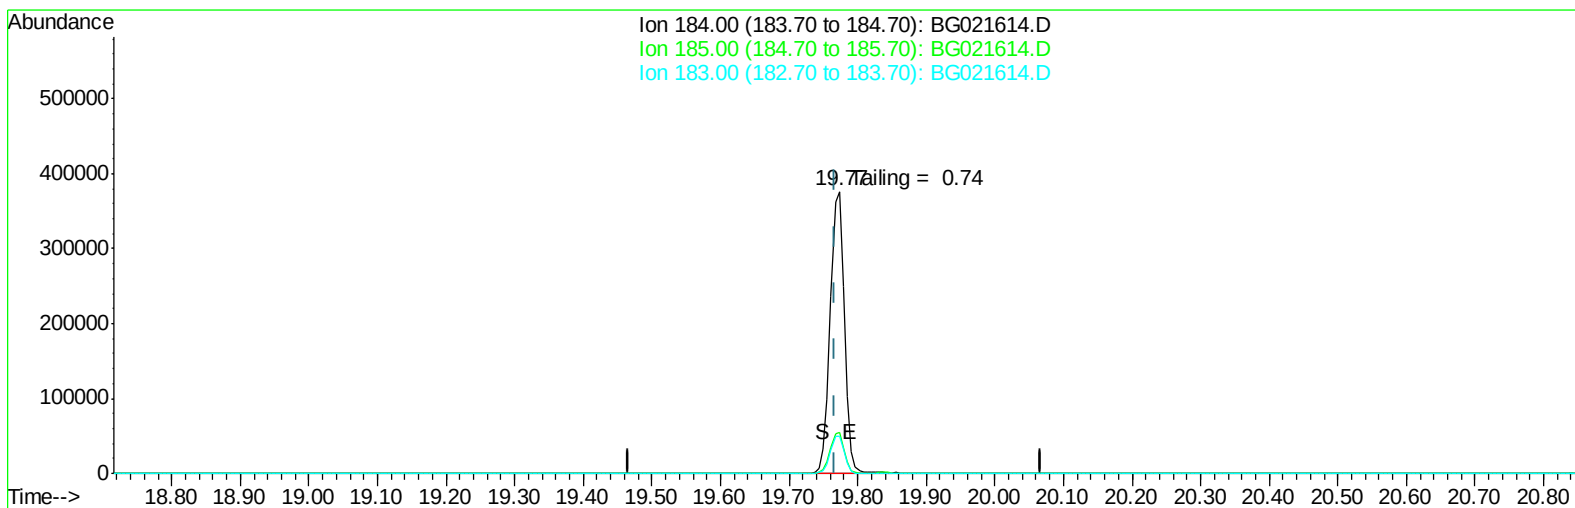

TIC: BG021614.D

(76) Benzidine

19.773min (+0.006) 17443.16ng

response 536040

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.71
183.00	12.80	13.42
0.00	0.00	0.00