


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041316\
 Data File : BG021614.D
 Acq On : 13 Apr 2016 10:17
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 15:48:13 2016

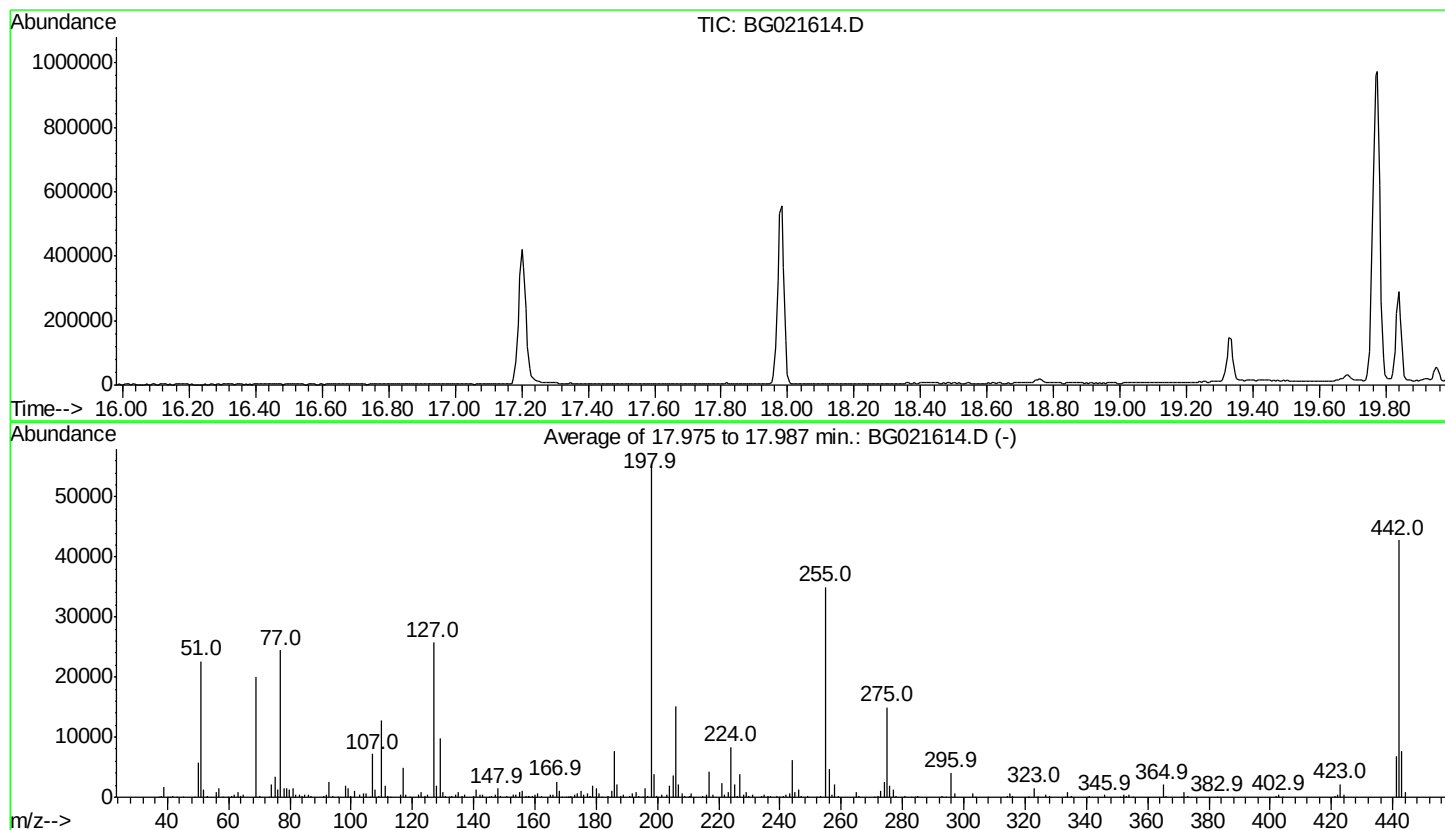

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	22669	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.5	20134	PASS
70	69	0.00	2	0.6	129	PASS
127	198	10	80	46.6	25741	PASS
197	198	0.00	2	0.2	133	PASS
198	198	100	100	100.0	55189	PASS
199	198	5	9	6.8	3773	PASS
275	198	10	60	27.2	15008	PASS
365	198	1	100	3.7	2059	PASS
441	442	0.01	24	15.9	6801	PASS
442	198	50	100	77.6	42802	PASS
443	442	15	24	17.9	7649	PASS