


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041316\
 Data File : BG021627.D
 Acq On : 13 Apr 2016 18:53
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 15:48:13 2016

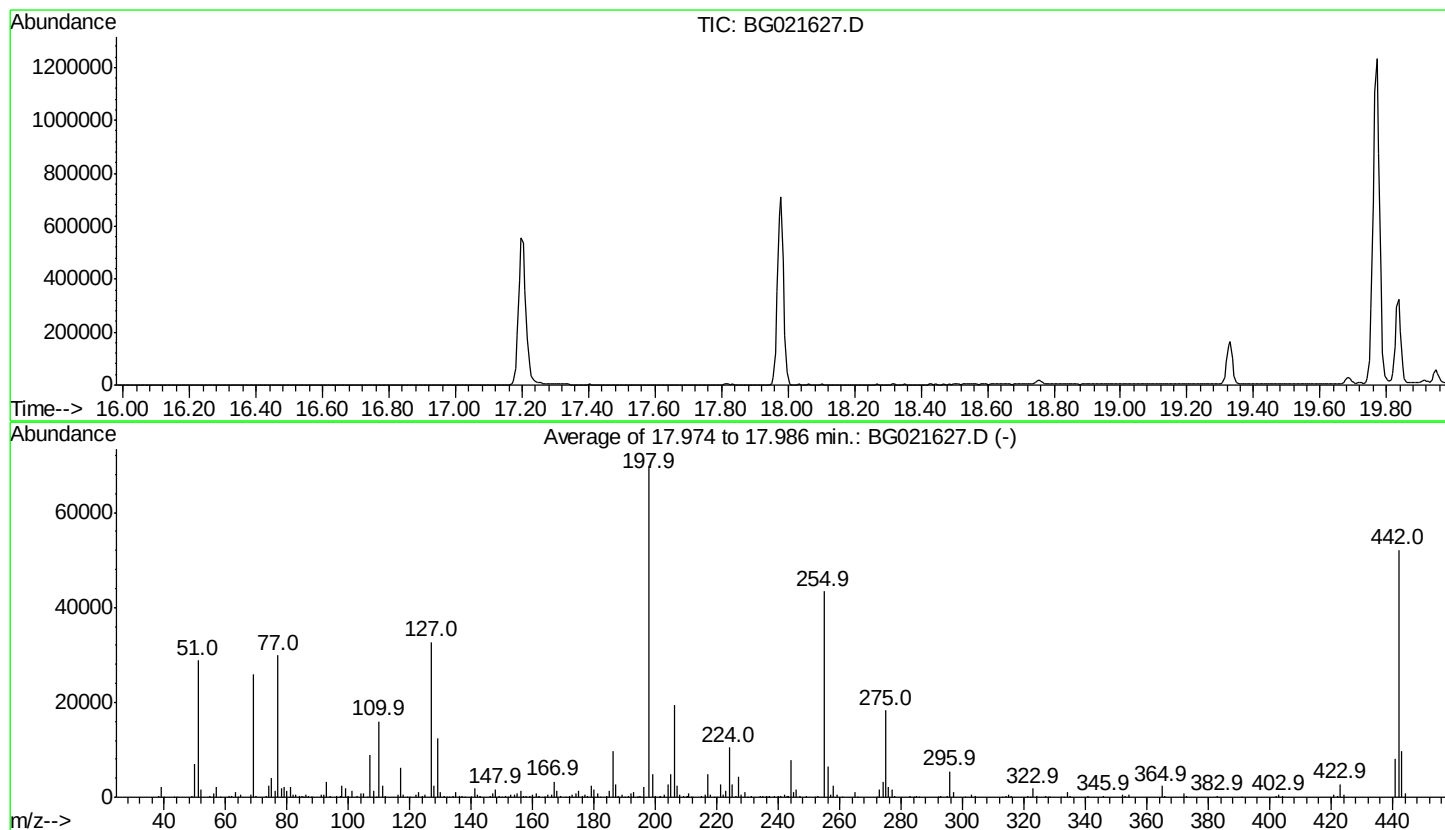

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	28818	PASS
68	69	0.00	2	2.0	515	PASS
69	198	0.00	100	37.1	25896	PASS
70	69	0.00	2	0.6	148	PASS
127	198	10	80	46.9	32770	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69866	PASS
199	198	5	9	7.0	4873	PASS
275	198	10	60	26.2	18306	PASS
365	198	1	100	3.4	2410	PASS
441	442	0.01	24	15.8	8230	PASS
442	198	50	100	74.7	52170	PASS
443	442	15	24	18.9	9838	PASS