
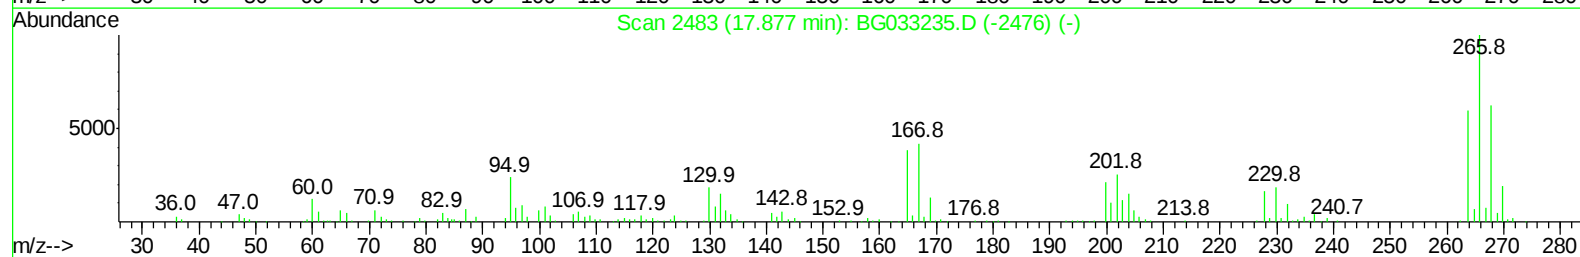
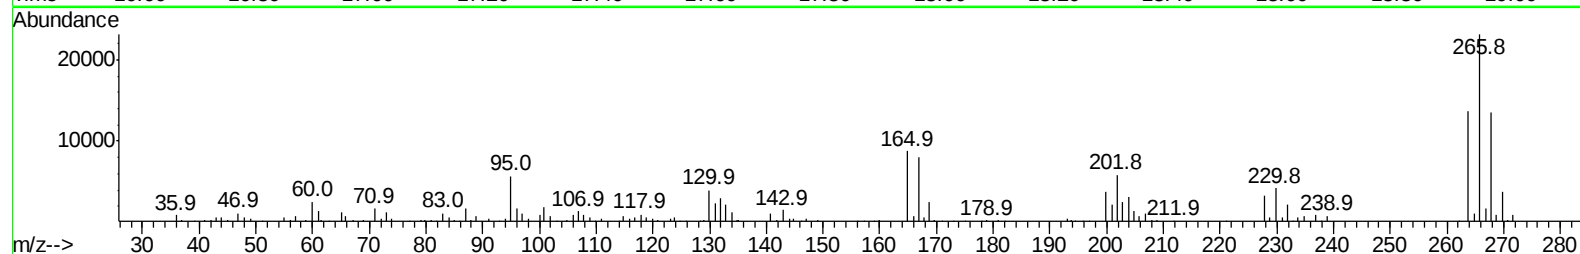


Data Path : Z:\HPCHEM1\BNA G\Data\BG041318\
Data File : BG033792.D
Acq On : 13 Apr 2018 10:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 03:52:42 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 16:51:36 2018
Response via : Initial Calibration

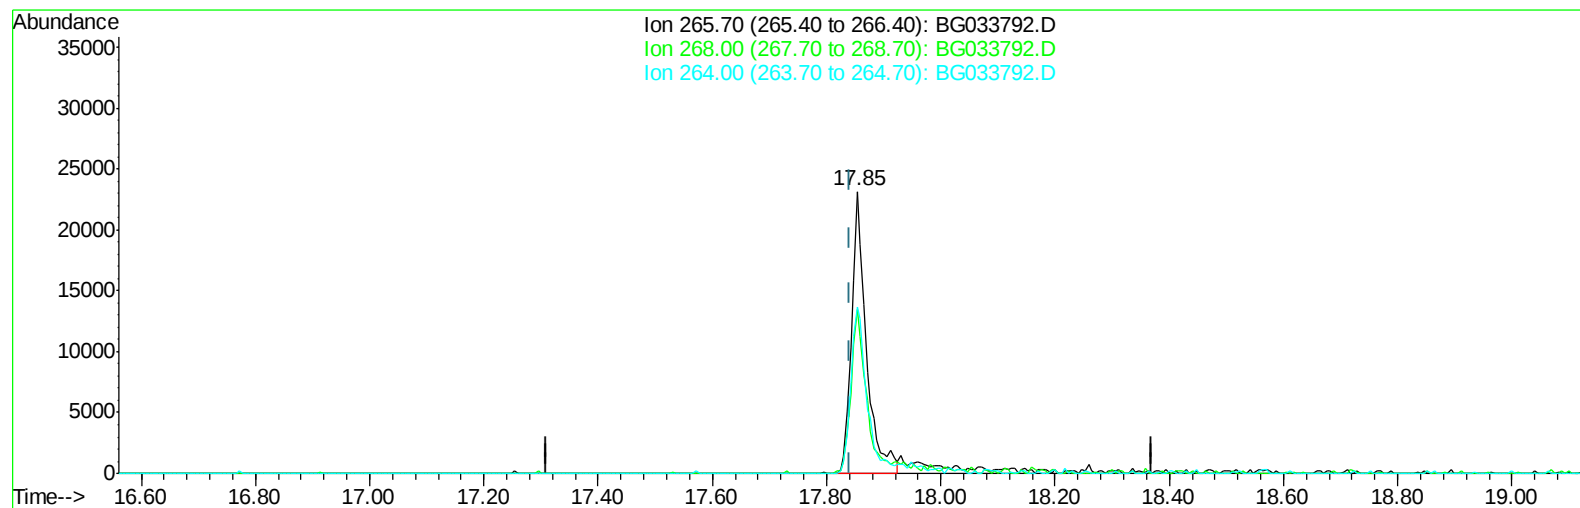

TIC: BG033792.D

(69) Pentachlorophenol (C)




17.853min (+0.012) 83416.20ng

response 41867

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.31
264.00	62.00	58.88
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG041318\
Data File : BG033792.D
Acq On : 13 Apr 2018 10:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 03:52:42 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 16:51:36 2018
Response via : Initial Calibration

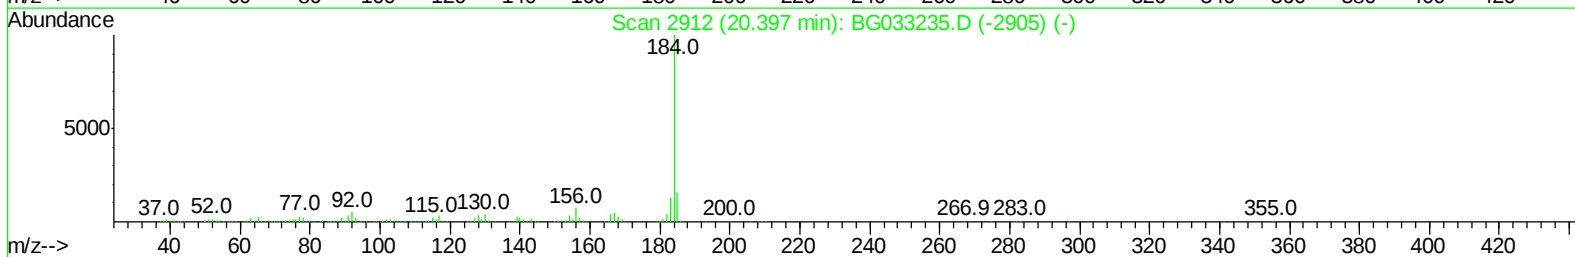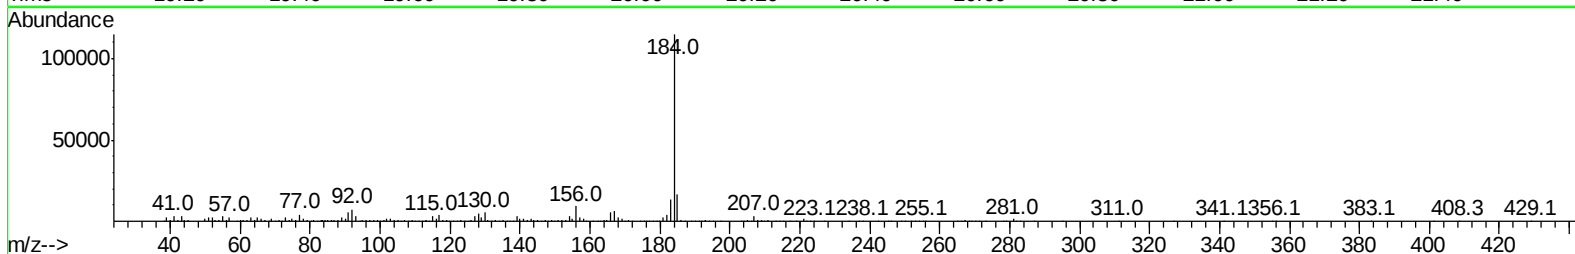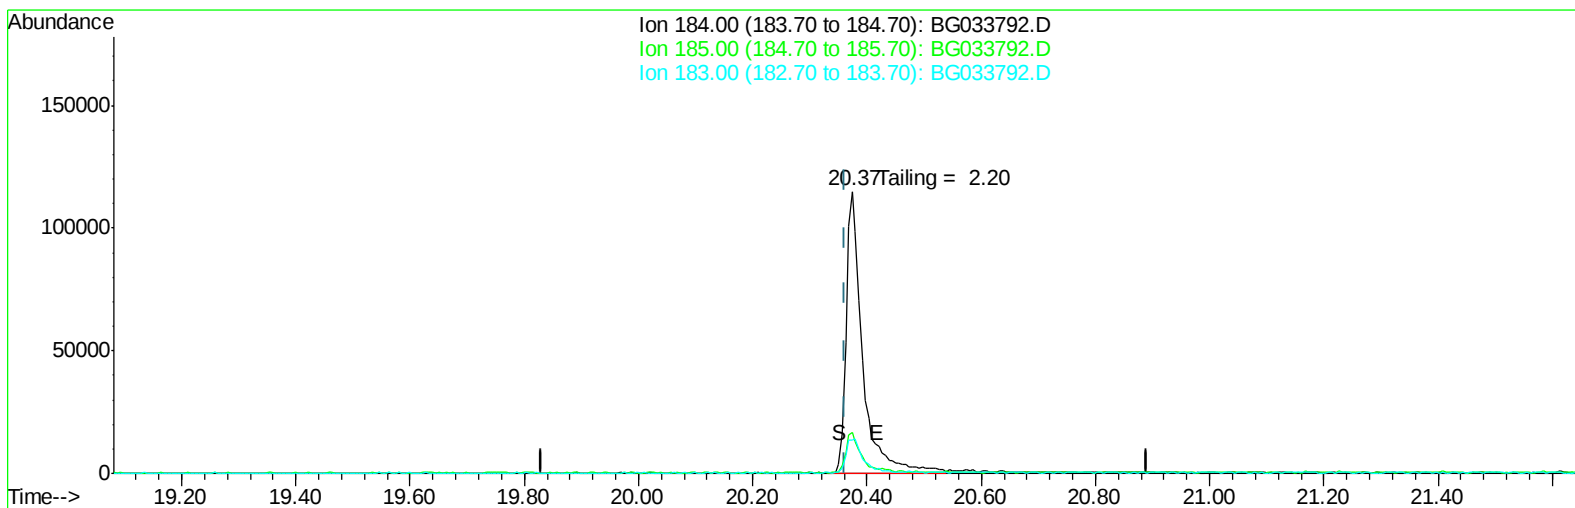

TIC: BG033792.D

(76) Benzidine

20.374min (+0.012) 36396.72ng

response 232938

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.63
183.00	13.30	12.03
0.00	0.00	0.00