


Data Path : Z:\HPCHEM1\BNA G\Data\BG041318\
 Data File : BG033792.D
 Acq On : 13 Apr 2018 10:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 16 11:44:01 2018

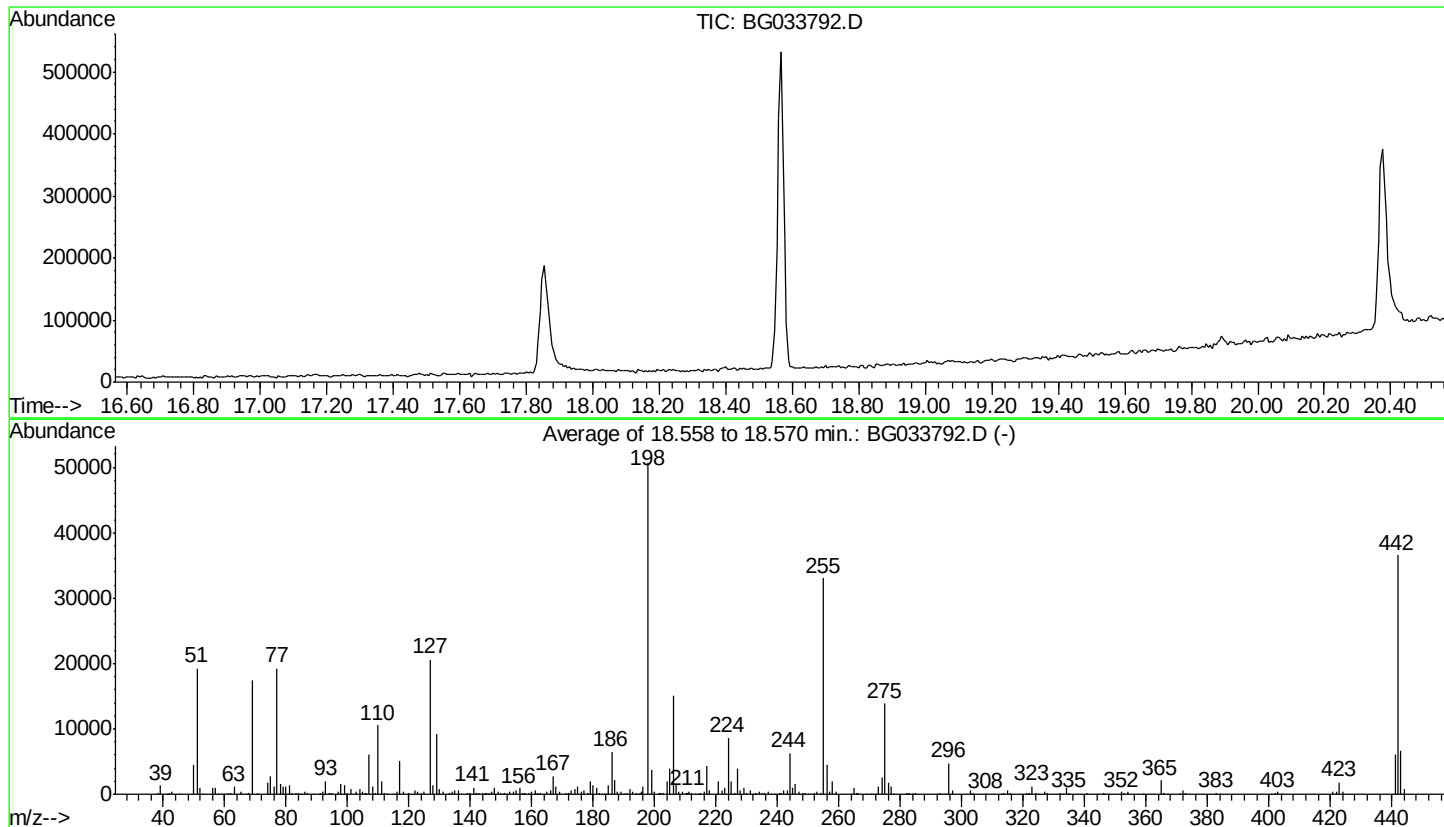

AutoFind: Scans 2599, 2600, 2601; Background Corrected with Scan 2593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	19265	PASS
68	69	0.00	2	1.0	168	PASS
69	198	0.00	100	34.2	17342	PASS
70	69	0.00	2	0.4	75	PASS
127	198	10	80	40.6	20608	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50720	PASS
199	198	5	9	7.3	3694	PASS
275	198	10	60	27.4	13884	PASS
365	198	1	100	4.2	2124	PASS
441	443	0.01	100	90.3	6017	PASS
442	198	50	100	72.1	36573	PASS
443	442	15	24	18.2	6662	PASS