

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041322\  
 Data File : BG053142.D  
 Acq On : 13 Apr 2022 17:25  
 Operator : CG/JU  
 Sample : N2368-05  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 FIELD-BLANK

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG040822.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053142.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.684       | 384           | 391         | 401          | rBV      | 328279         | 538578        | 14.12%          | 4.127%        |
| 2         | 7.276       | 655           | 662         | 671          | rBV2     | 206924         | 368536        | 9.66%           | 2.824%        |
| 3         | 8.122       | 797           | 806         | 812          | rBV      | 125693         | 217833        | 5.71%           | 1.669%        |
| 4         | 9.279       | 995           | 1003        | 1012         | rBV      | 516420         | 952741        | 24.98%          | 7.300%        |
| 5         | 10.930      | 1278          | 1284        | 1293         | rVB      | 167178         | 305370        | 8.01%           | 2.340%        |
| 6         | 13.368      | 1692          | 1699        | 1709         | rBV      | 1435082        | 2246219       | 58.88%          | 17.211%       |
| 7         | 14.743      | 1925          | 1933        | 1941         | rBV      | 300827         | 472800        | 12.39%          | 3.623%        |
| 8         | 16.229      | 2179          | 2186        | 2203         | rBV      | 1346471        | 2091246       | 54.82%          | 16.024%       |
| 9         | 17.486      | 2394          | 2400        | 2407         | rBV      | 420835         | 643208        | 16.86%          | 4.929%        |
| 10        | 20.088      | 2837          | 2843        | 2849         | rBV      | 2918619        | 3814681       | 100.00%         | 29.230%       |
| 11        | 21.768      | 3122          | 3129        | 3136         | rBV      | 418782         | 698845        | 18.32%          | 5.355%        |
| 12        | 25.064      | 3680          | 3690        | 3702         | rBV2     | 237618         | 700657        | 18.37%          | 5.369%        |




Sum of corrected areas: 13050714

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041322\  
Data File : BG053142.D  
Acq On : 13 Apr 2022 17:25  
Operator : CG/JU  
Sample : N2368-05  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
FIELD-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG040822.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

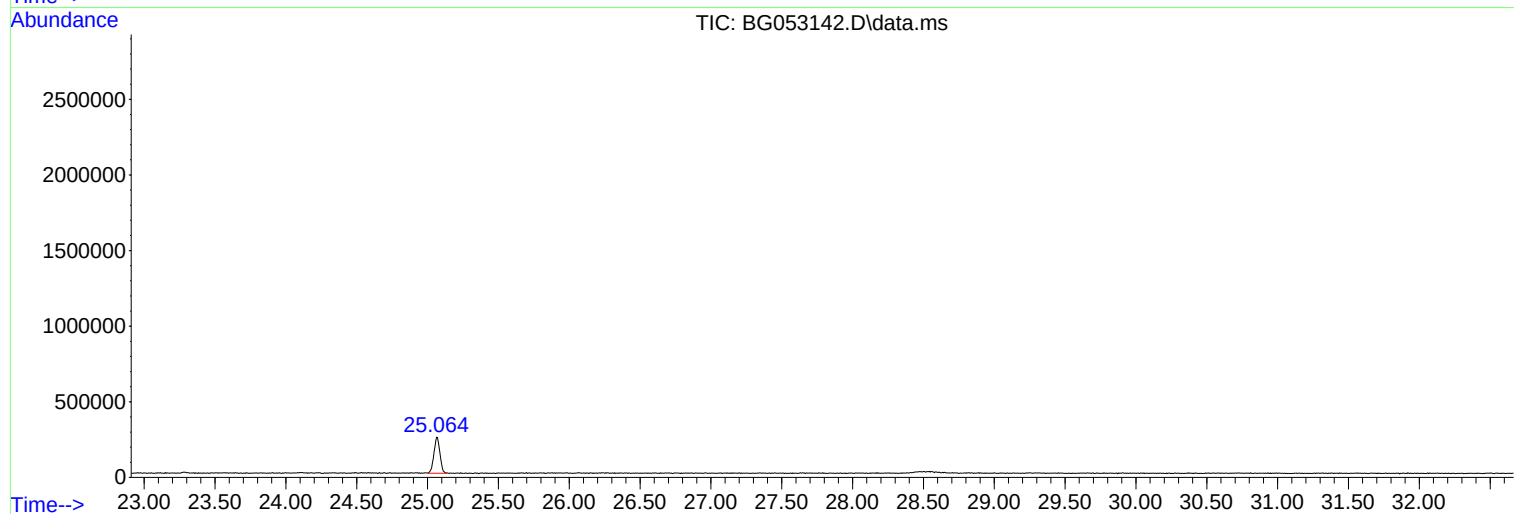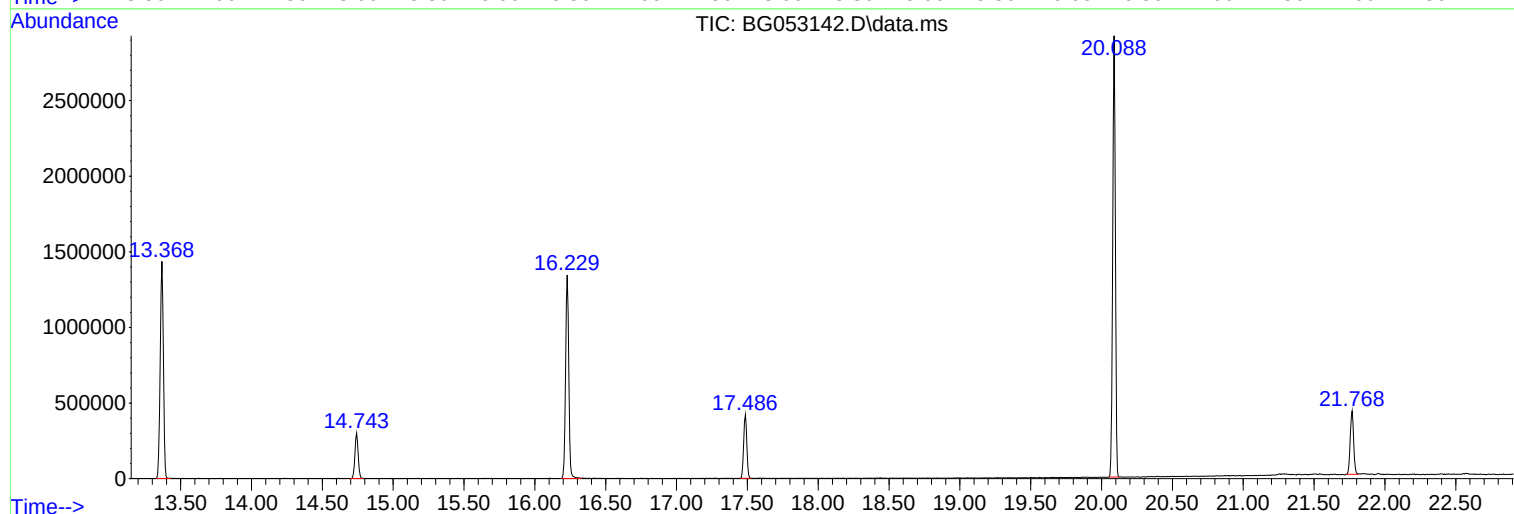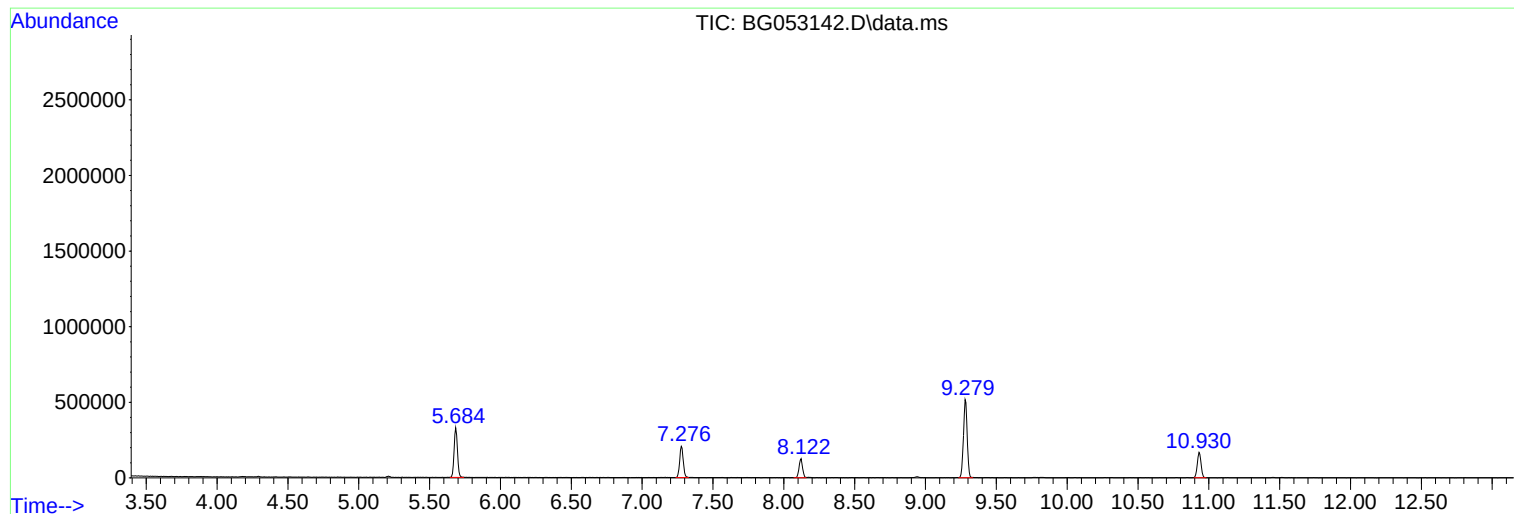

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041322\  
Data File : BG053142.D  
Acq On : 13 Apr 2022 17:25  
Operator : CG/JU  
Sample : N2368-05  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
FIELD-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG040822.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041322\  
Data File : BG053142.D  
Acq On : 13 Apr 2022 17:25  
Operator : CG/JU  
Sample : N2368-05  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
FIELD-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG040822.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|