
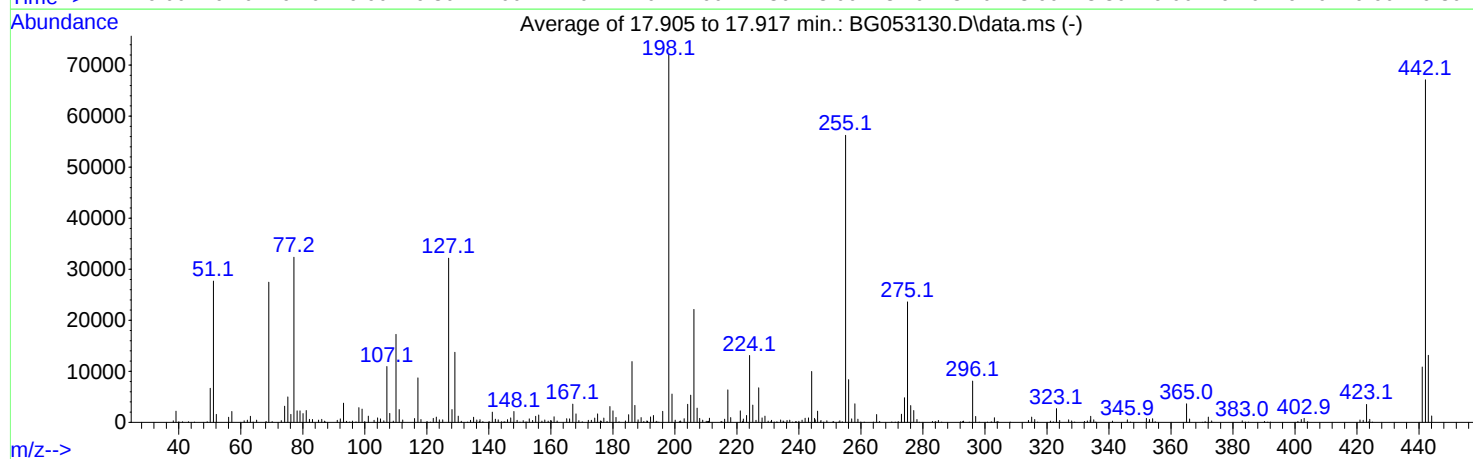


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041322\
 Data File : BG053130.D
 Acq On : 13 Apr 2022 9:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 15:31:24 2022

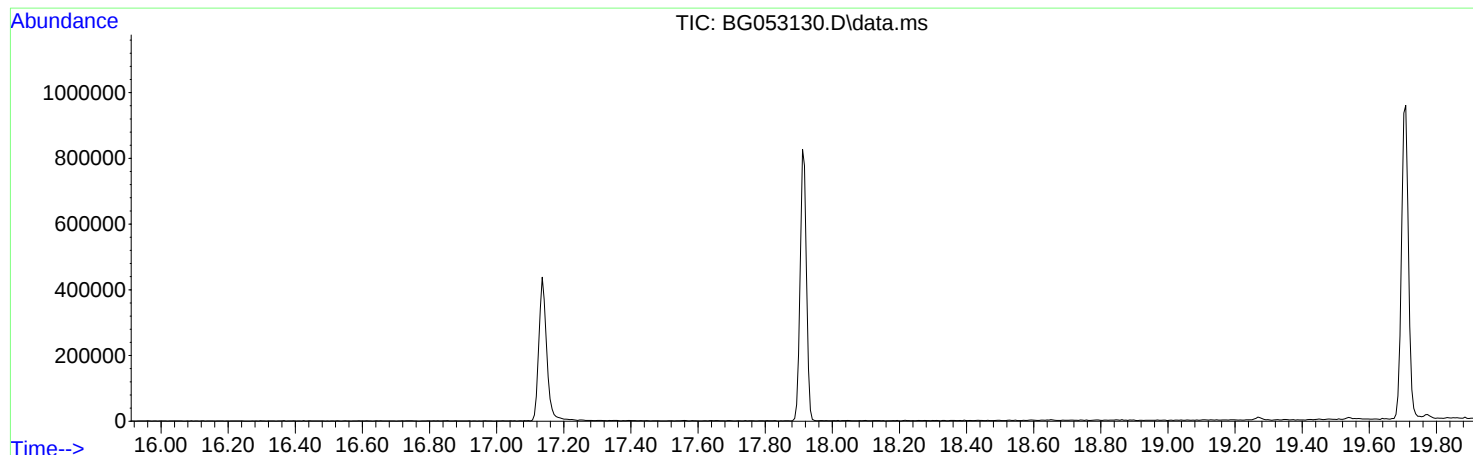




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	27683	PASS
68	69	0.00	2	0.7	202	PASS
69	198	0.00	100	38.1	27472	PASS
70	69	0.00	2	0.6	158	PASS
127	198	10	80	44.6	32176	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72080	PASS
199	198	5	9	7.7	5565	PASS
275	198	10	60	32.8	23621	PASS
365	198	1	100	5.0	3639	PASS
441	198	0.01	100	15.1	10864	PASS
442	442	50	100	100.0	67141	PASS
443	442	15	24	19.6	13127	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041322\
Data File : BG053130.D
Acq On : 13 Apr 2022 9:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 14 05:27:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

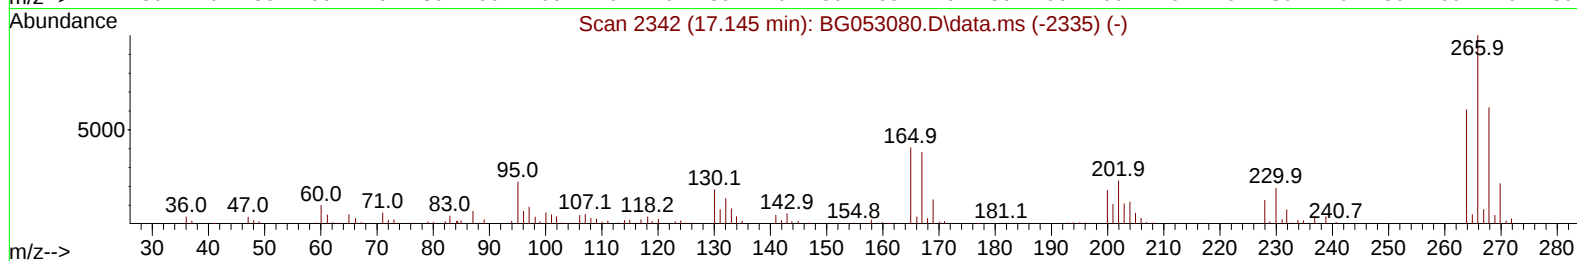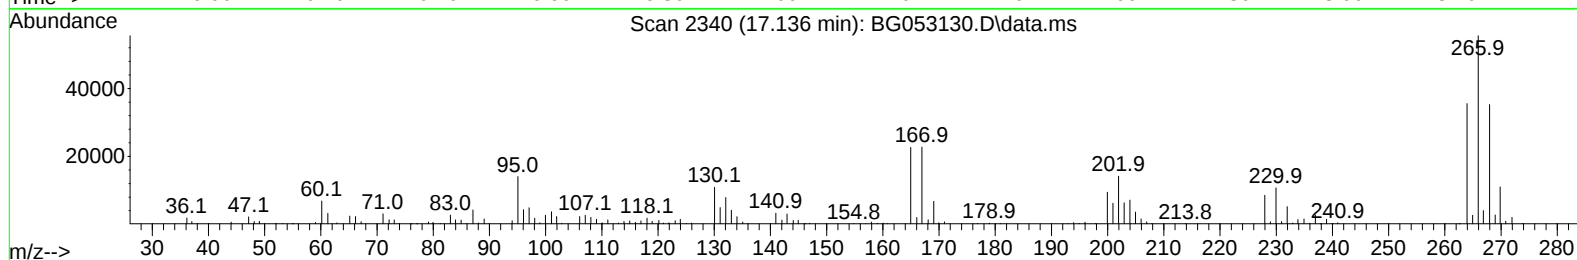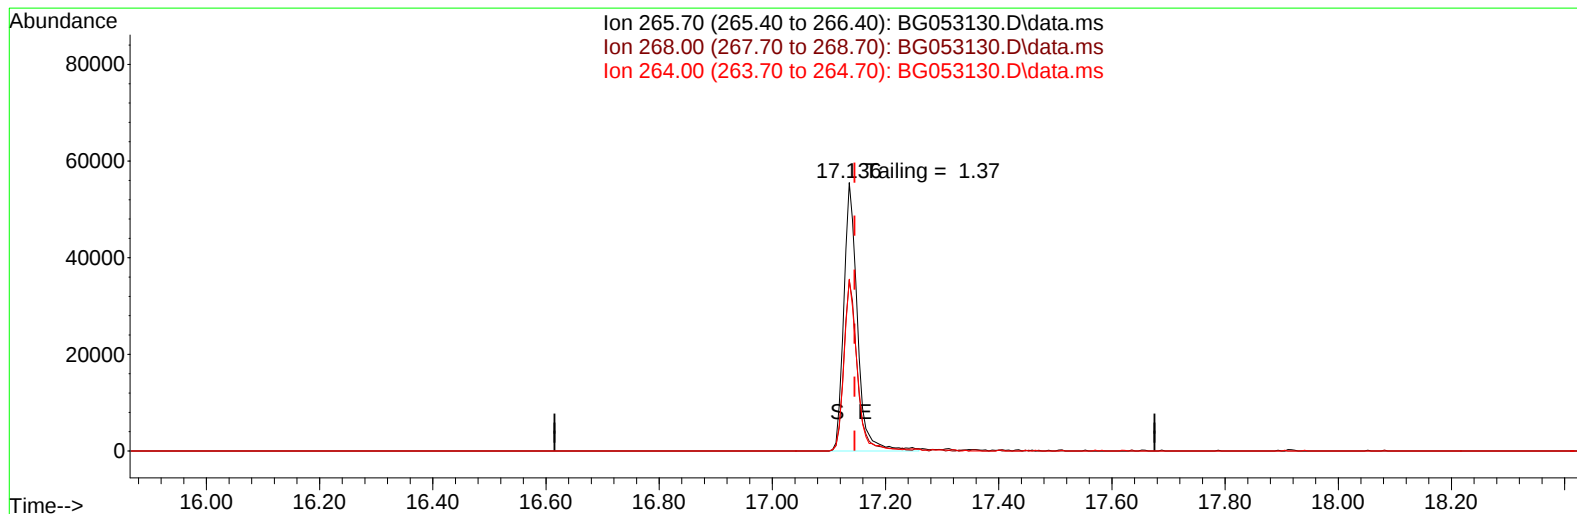

TIC: BG053130.D\data.ms

(70) Pentachlorophenol (C)

17.136min (-0.009) 20694.55 ng




response 92126

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	63.54
264.00	56.60	64.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041322\
Data File : BG053130.D
Acq On : 13 Apr 2022 9:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 14 05:27:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

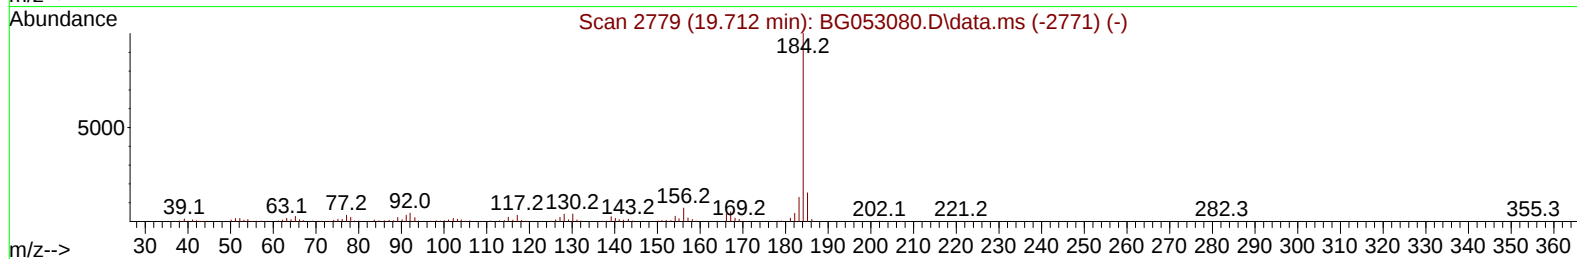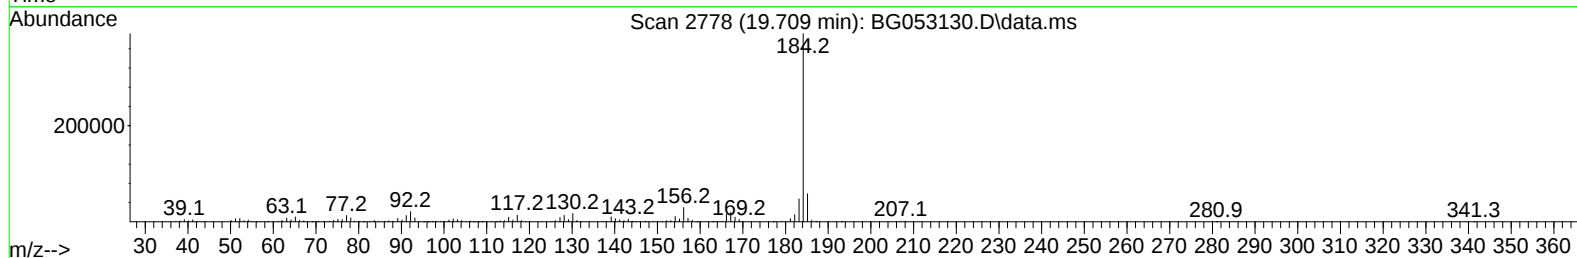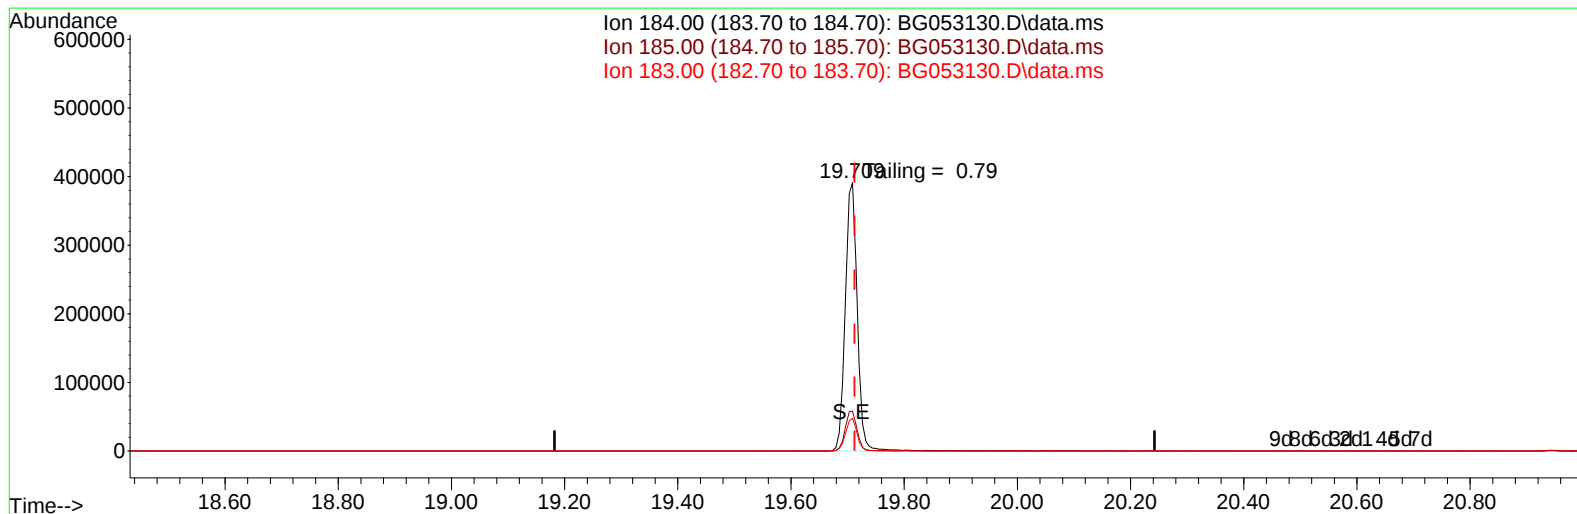

TIC: BG053130.D\data.ms

(77) Benzidine

19.709min (-0.003) 358159.32 ng m

response 572256

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.90
183.00	11.80	12.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/13/2022	BNA_G	BG053130.D
Compound Name	Response	Retention Time
DDT	299013	20.942
DDD	3664	20.502
DDE	593	19.991
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4257	303270	1.40

Instrument :
BNA_G
ClientSampleId :
DFTPP