


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041323\
Data File : BG057077.D
Acq On : 13 Apr 2023 10:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 13 05:15:23 2023

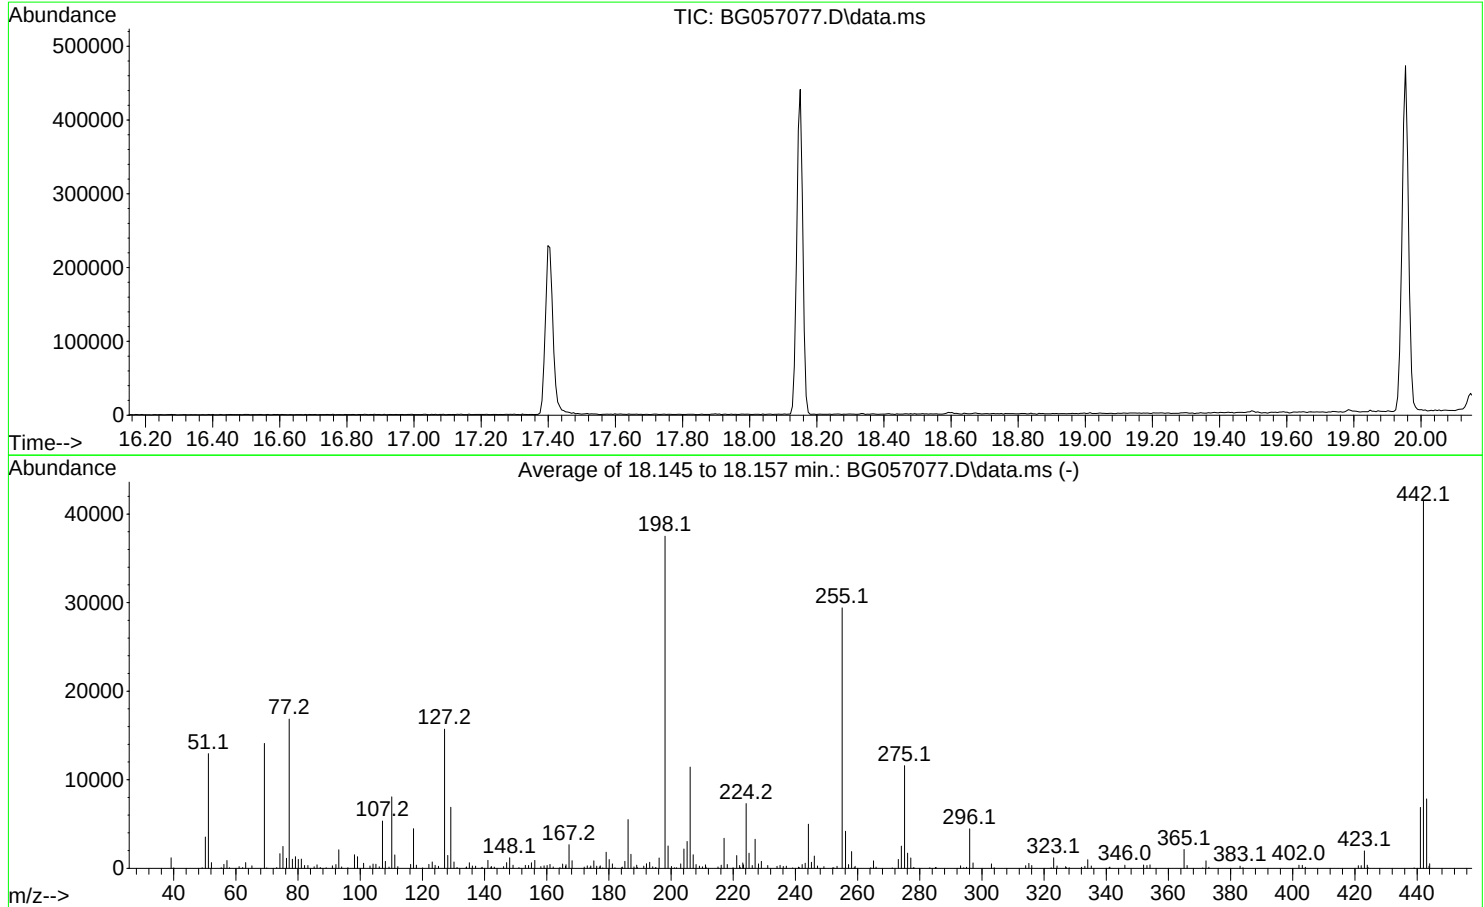




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	12955	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.6	14111	PASS
70	69	0.00	2	0.4	51	PASS
127	198	10	80	41.9	15709	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37509	PASS
199	198	5	9	6.7	2524	PASS
275	198	10	60	30.9	11589	PASS
365	198	1	100	5.7	2131	PASS
441	198	0.01	100	18.3	6873	PASS
442	442	50	100	100.0	41539	PASS
443	442	15	24	18.8	7829	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041323\
Data File : BG057077.D
Acq On : 13 Apr 2023 10:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 13 13:46:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:15:23 2023
Response via : Initial Calibration

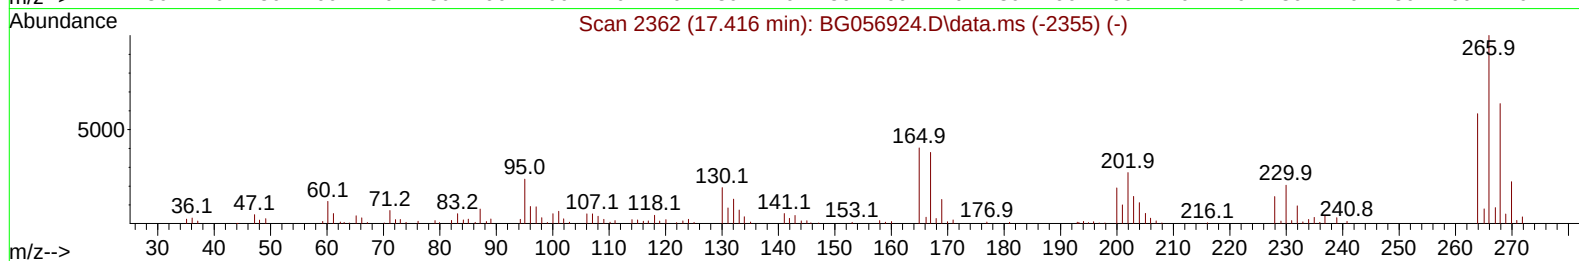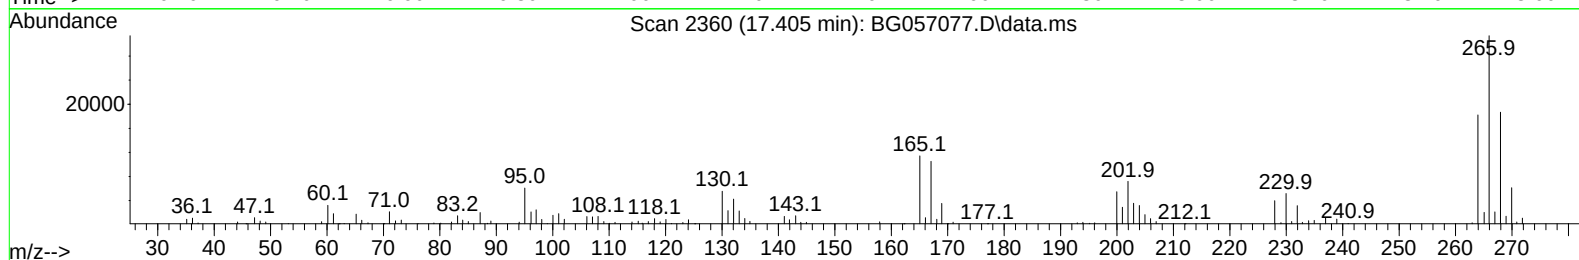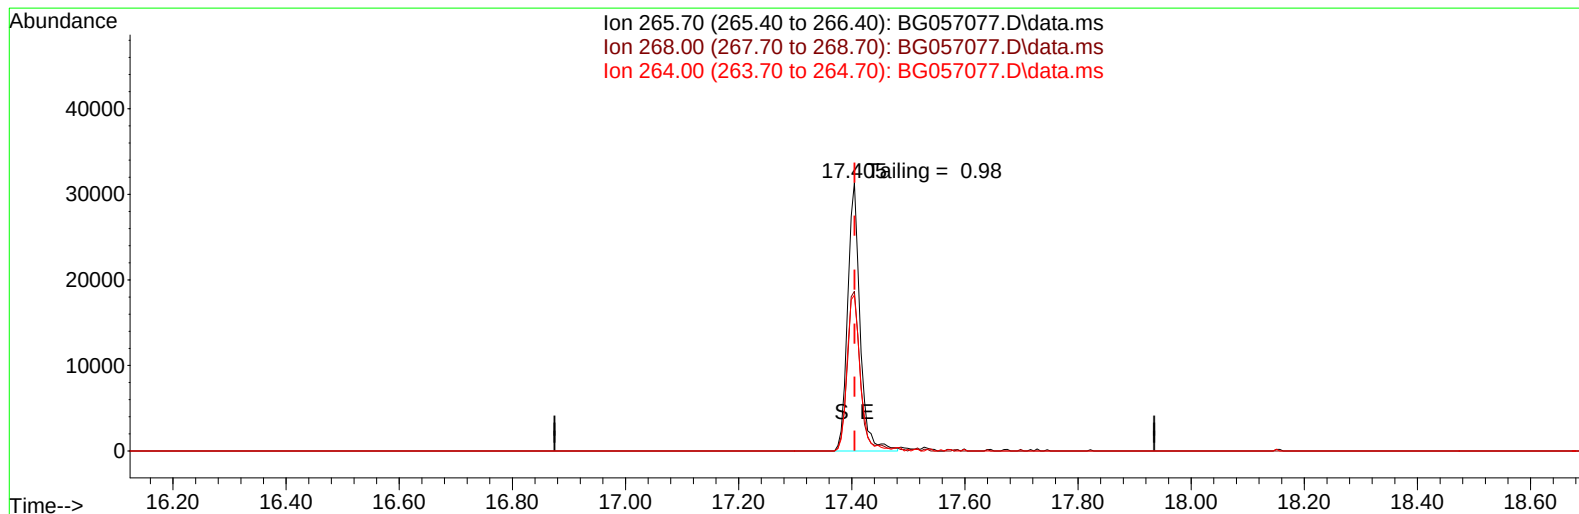

TIC: BG057077.D\data.ms

(70) Pentachlorophenol (C)

17.405min (-0.000) 101090.04 ng




response 47907

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	59.53
264.00	58.50	58.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041323\
Data File : BG057077.D
Acq On : 13 Apr 2023 10:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 13 13:46:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:15:23 2023
Response via : Initial Calibration

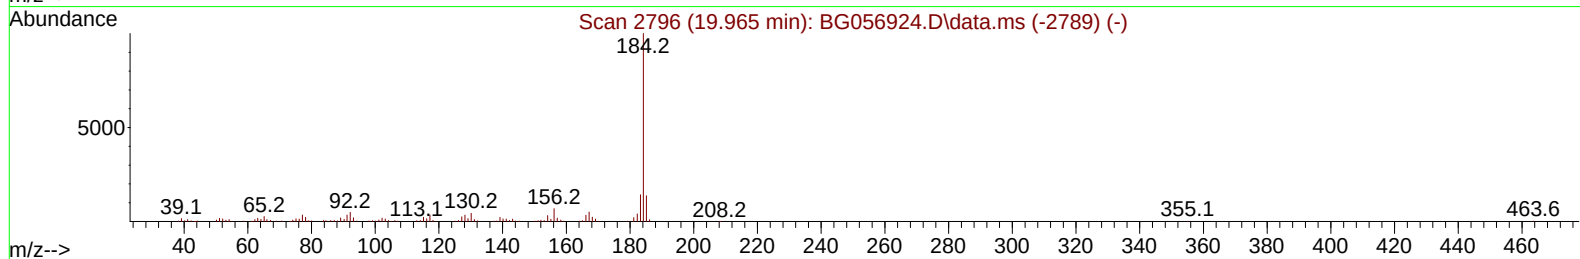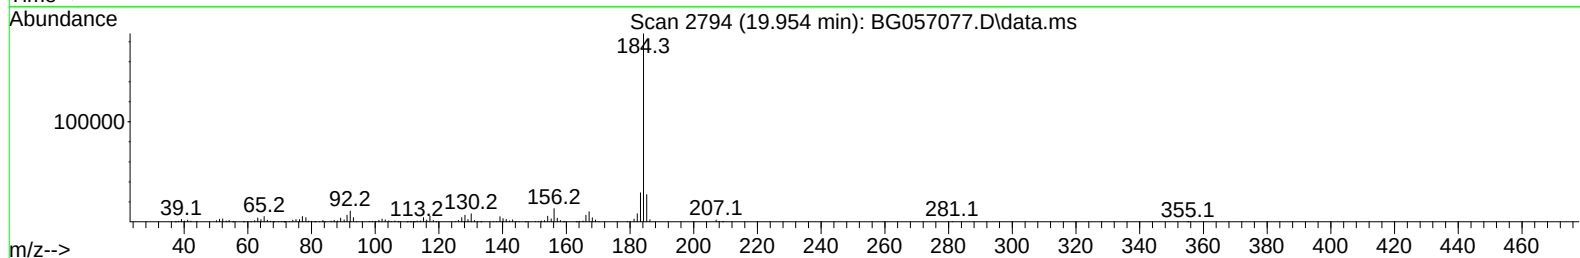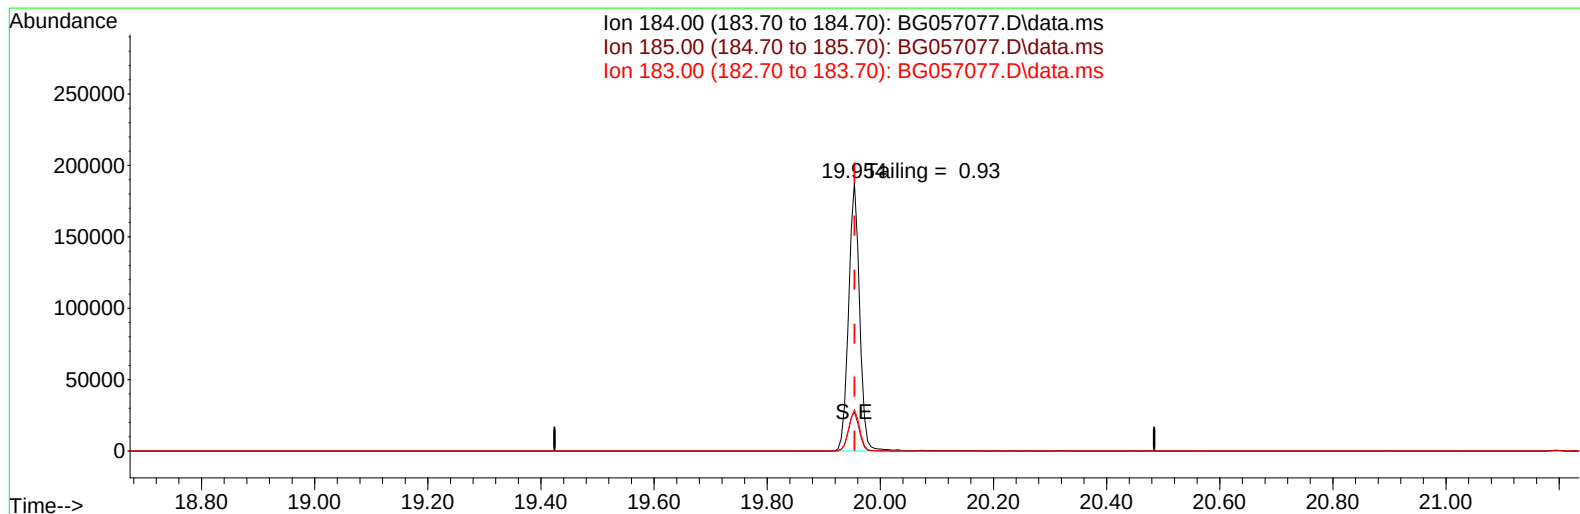

TIC: BG057077.D\data.ms

(77) Benzidine

19.954min (-0.000) 2219.26 ng

response 254831

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.54
183.00	14.20	15.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/13/2023	BNA_G	<u>BG057077.D</u>
Compound Name	Response	Retention Time
DDT	131824	21.194
DDD	4199	20.73
DDE	0	20.233
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4199	136023	3.09

Instrument :
BNA_G
ClientSampleId :
DFTPP