
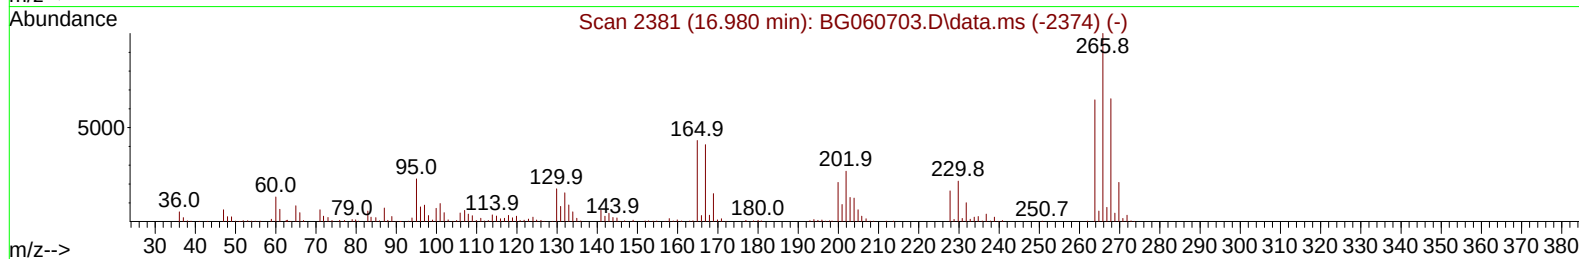
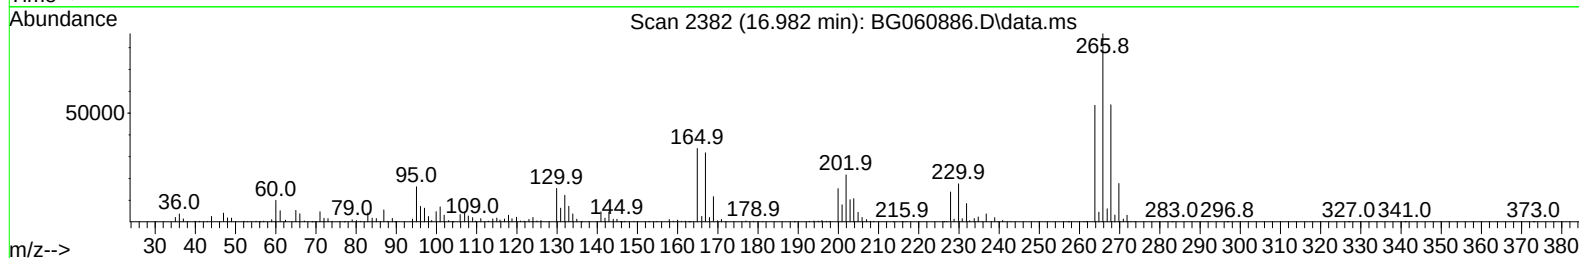


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041324\
Data File : BG060886.D
Acq On : 13 Apr 2024 9:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 01:12:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

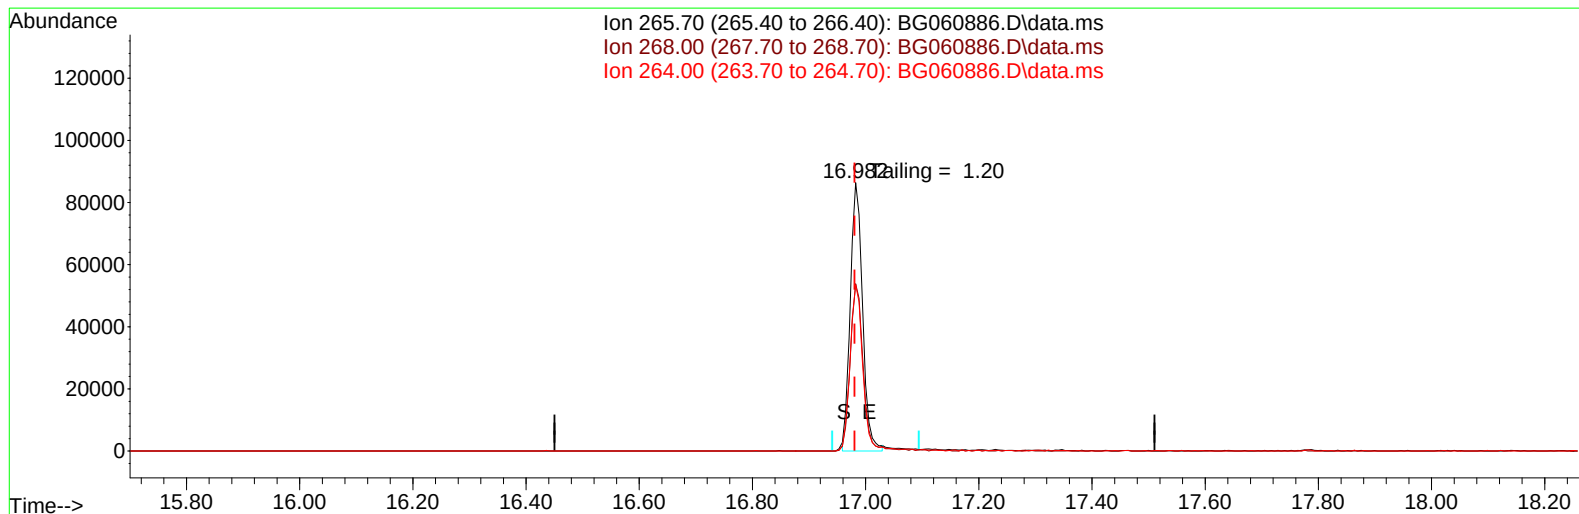

TIC: BG060886.D\data.ms

(70) Pentachlorophenol (C)




16.982min (+ 0.002) 326677.93 ng

response 134313

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.29
264.00	64.70	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041324\
Data File : BG060886.D
Acq On : 13 Apr 2024 9:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 01:12:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

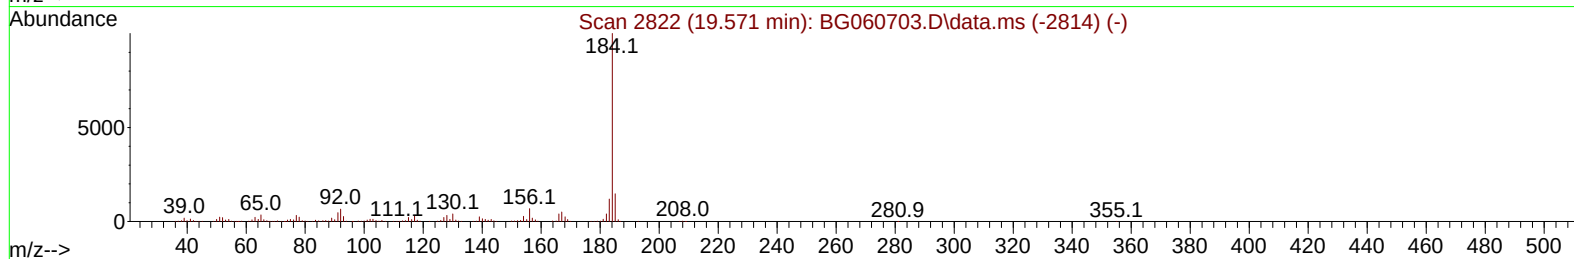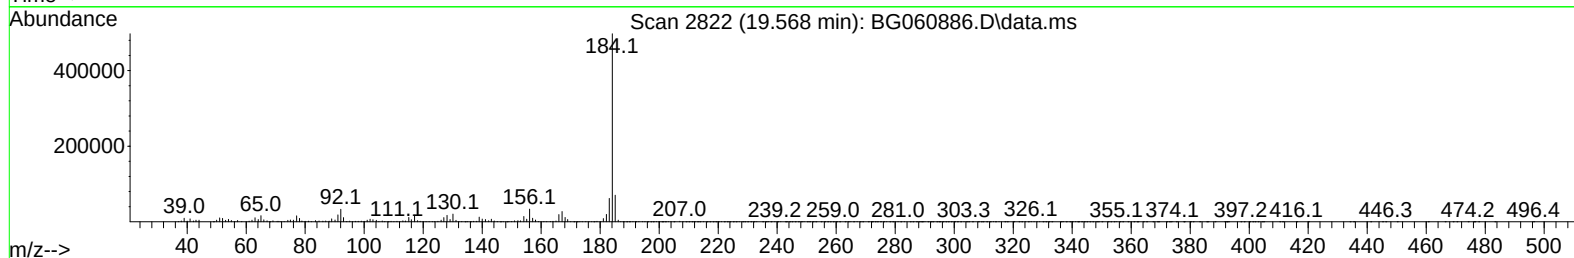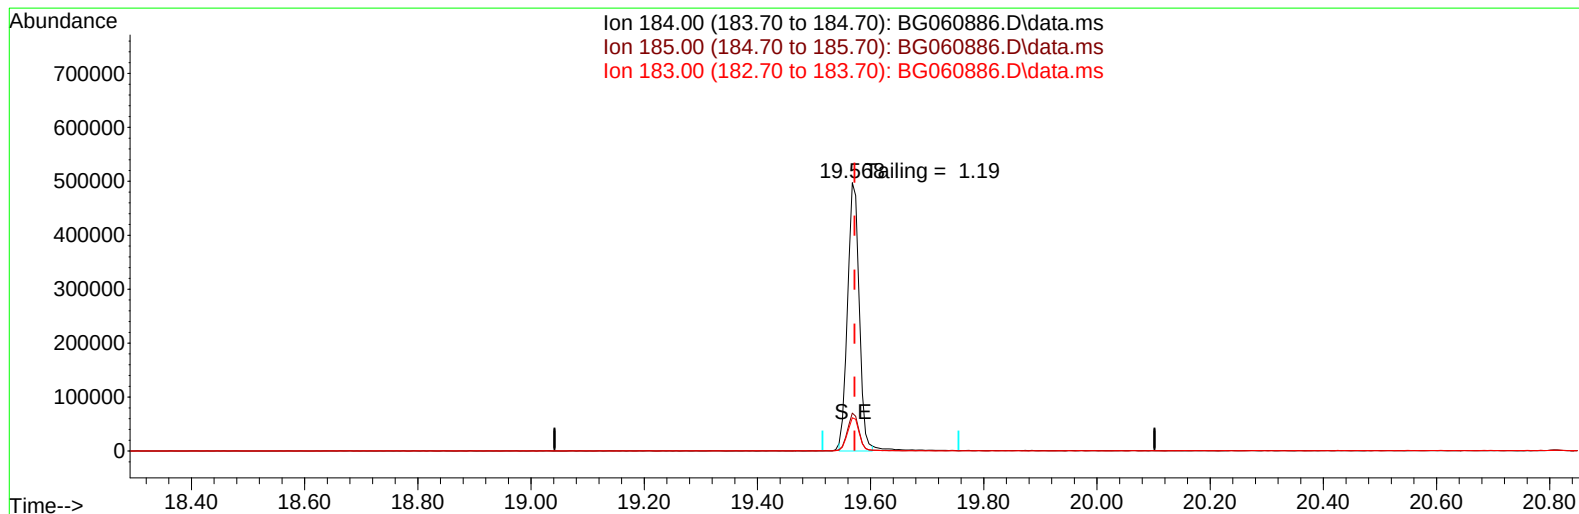

TIC: BG060886.D\data.ms

(77) Benzidine**19.568min (-0.004) 161960.35 ng****response 729275**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.12
183.00	11.90	12.45
0.00	0.00	0.00