
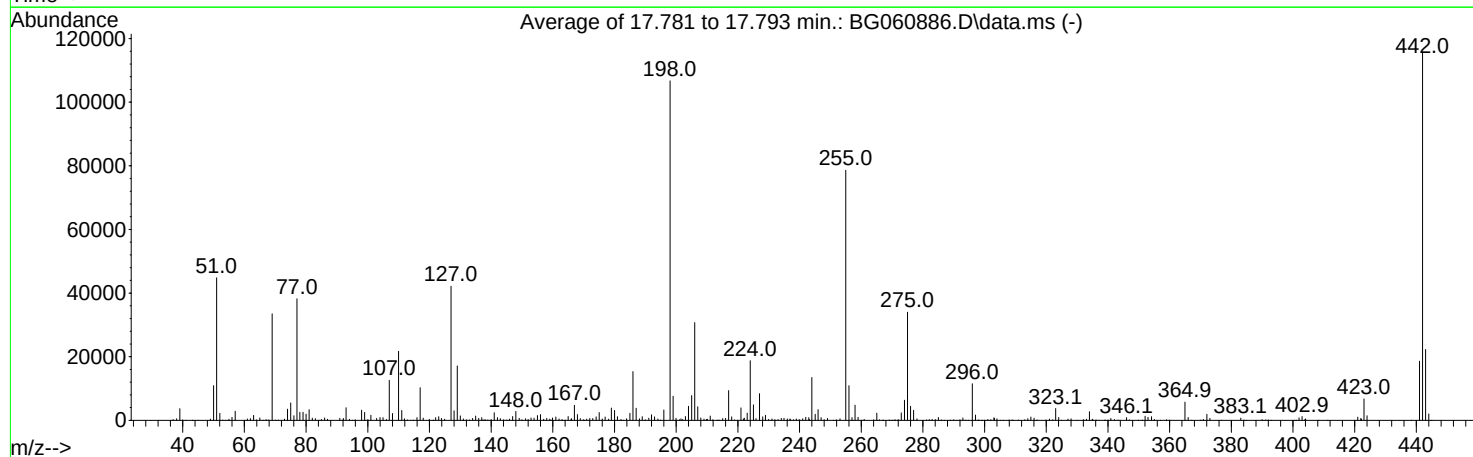


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041324\
Data File : BG060886.D
Acq On : 13 Apr 2024 9:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

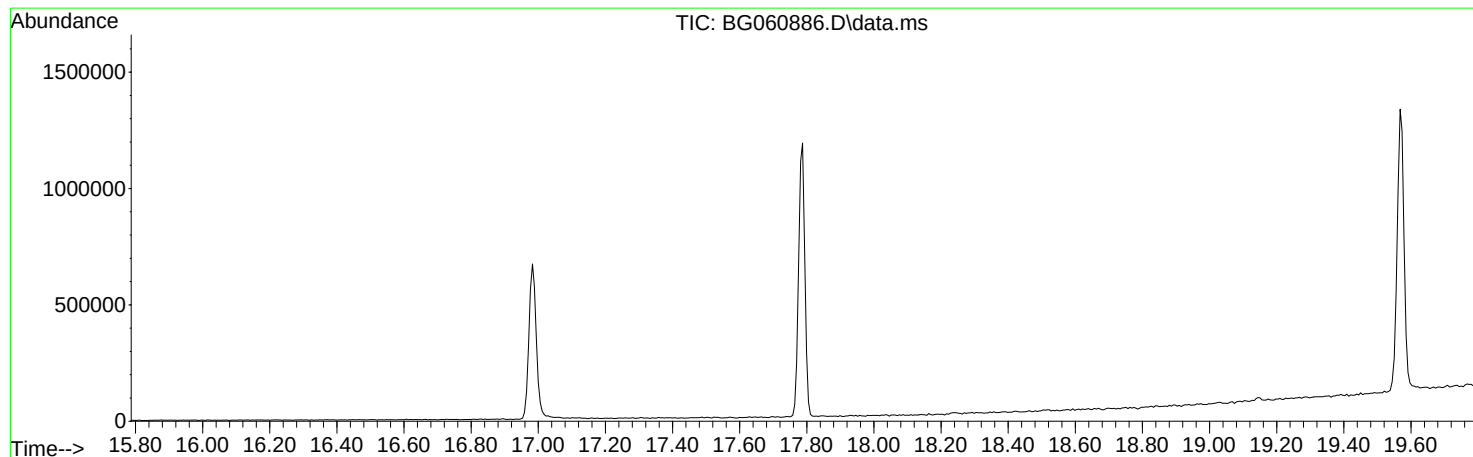




AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	44819	PASS
68	69	0.00	2	0.5	159	PASS
69	198	0.00	100	31.4	33484	PASS
70	69	0.00	2	0.3	97	PASS
127	198	10	80	39.5	42168	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106715	PASS
199	198	5	9	7.1	7577	PASS
275	198	10	60	31.9	34013	PASS
365	198	1	100	5.4	5713	PASS
441	198	0.01	100	17.4	18609	PASS
442	442	50	100	100.0	115616	PASS
443	442	15	24	19.3	22267	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041324\
Data File : BG060886.D
Acq On : 13 Apr 2024 9:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 15 01:12:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

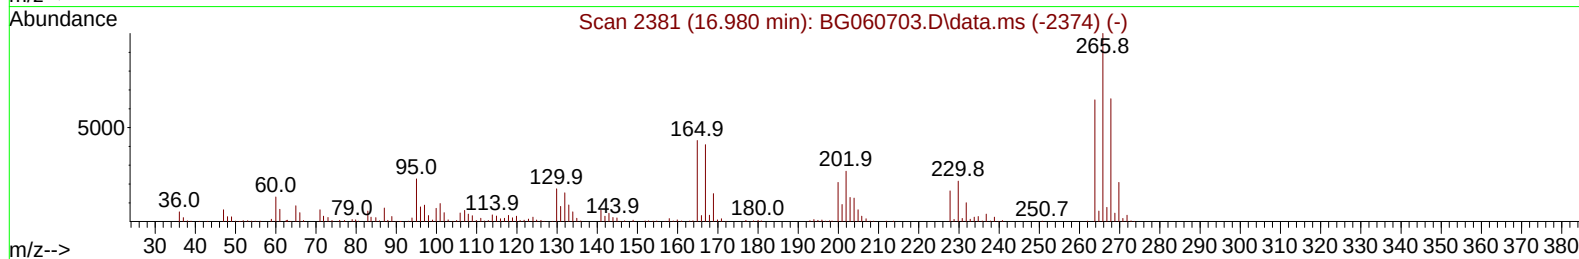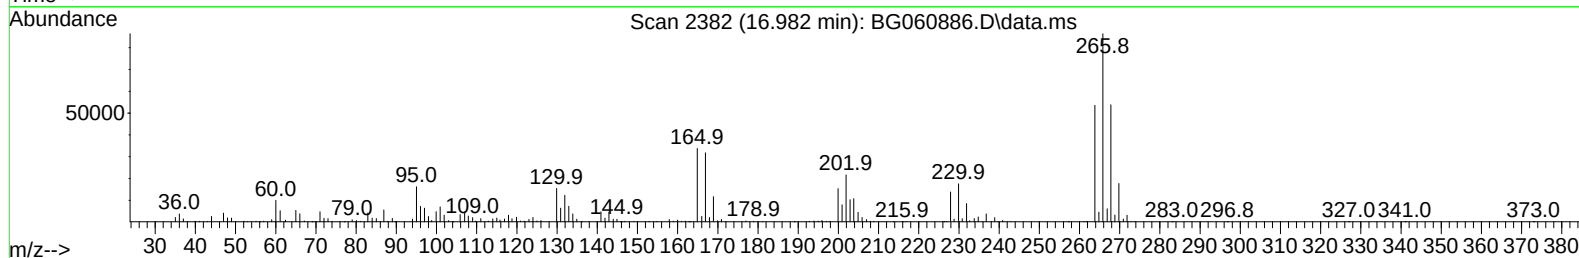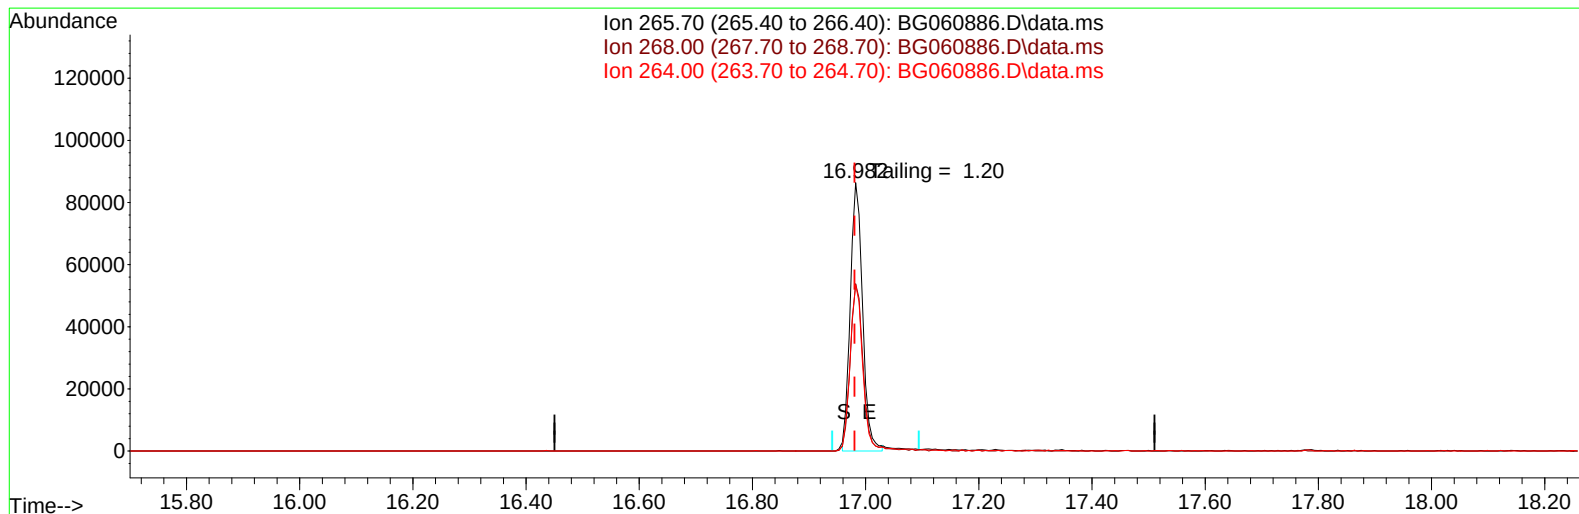

TIC: BG060886.D\data.ms

(70) Pentachlorophenol (C)

16.982min (+ 0.002) 326677.93 ng




response 134313

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.29
264.00	64.70	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041324\
Data File : BG060886.D
Acq On : 13 Apr 2024 9:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 15 01:12:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

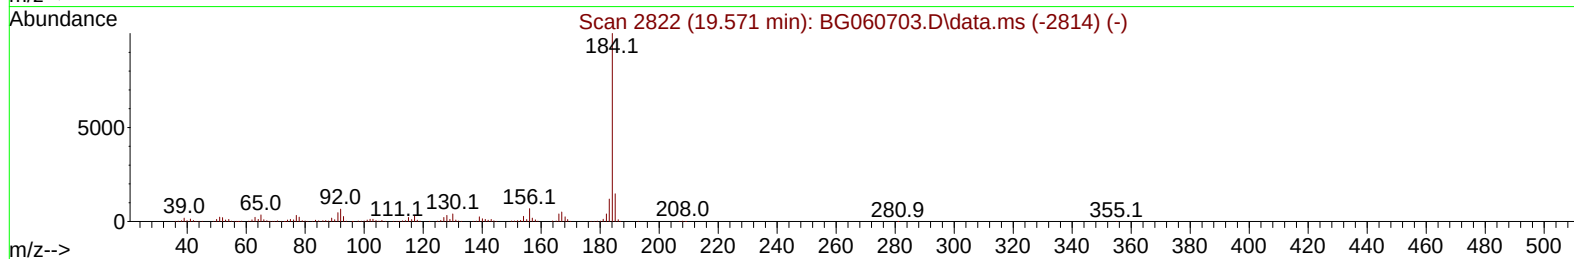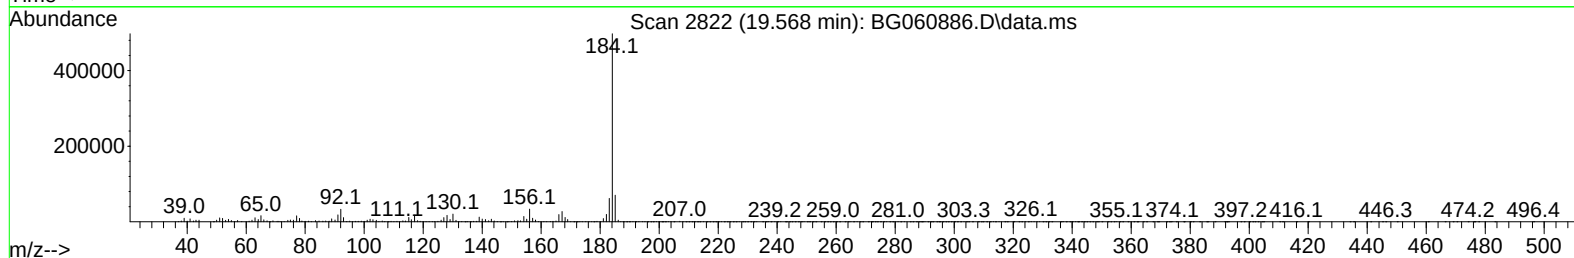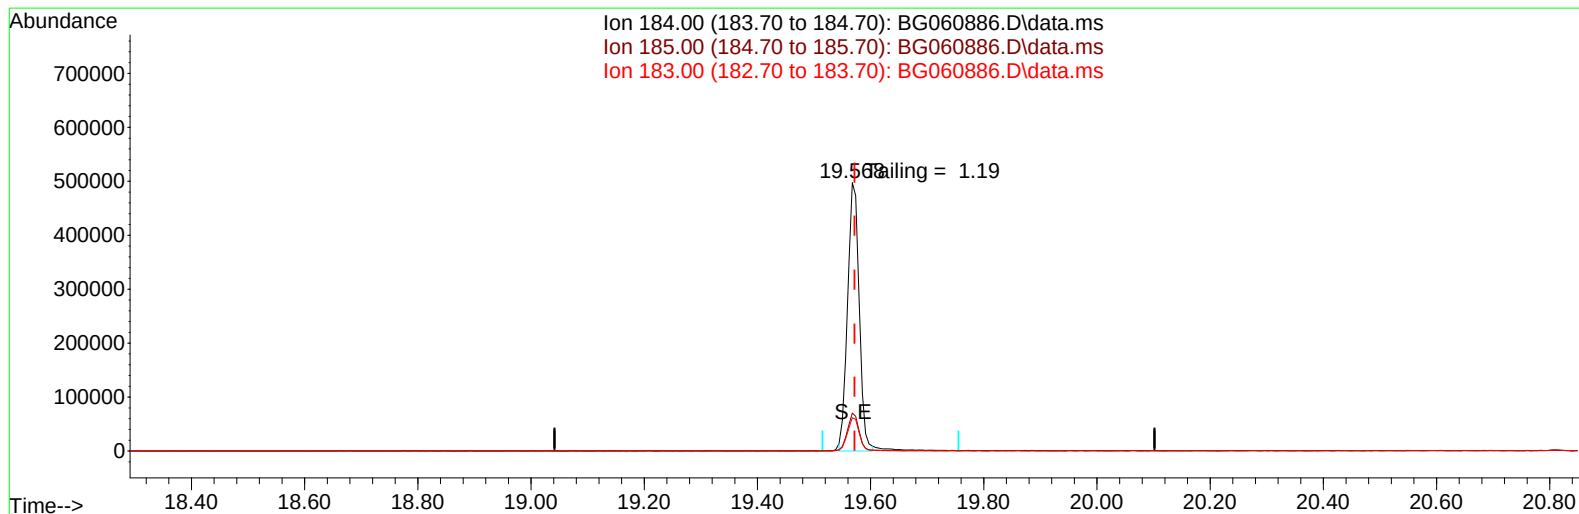

TIC: BG060886.D\data.ms

(77) Benzidine

19.568min (-0.004) 161960.35 ng

response 729275

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.12
183.00	11.90	12.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/13/2024	BNA_G	<u>BG060886.D</u>
Compound Name	Response	Retention Time
DDT	354890	20.813
DDD	15596	20.367
DDE	3278	19.867
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18874	373764	5.05

Instrument :
BNA_G
ClientSampleId :
DFTPP