
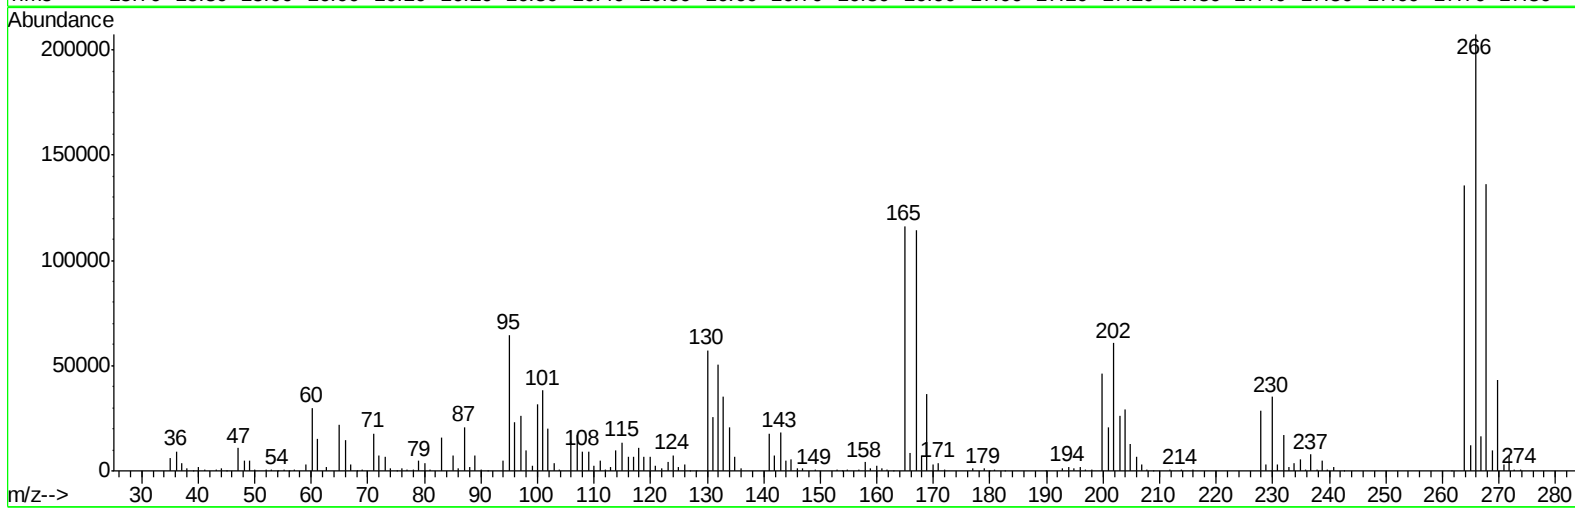


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041415\
Data File : BG016394.D
Acq On : 14 Apr 2015 13:45
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 06:57:32 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 14:00:56 2015
Response via : Initial Calibration

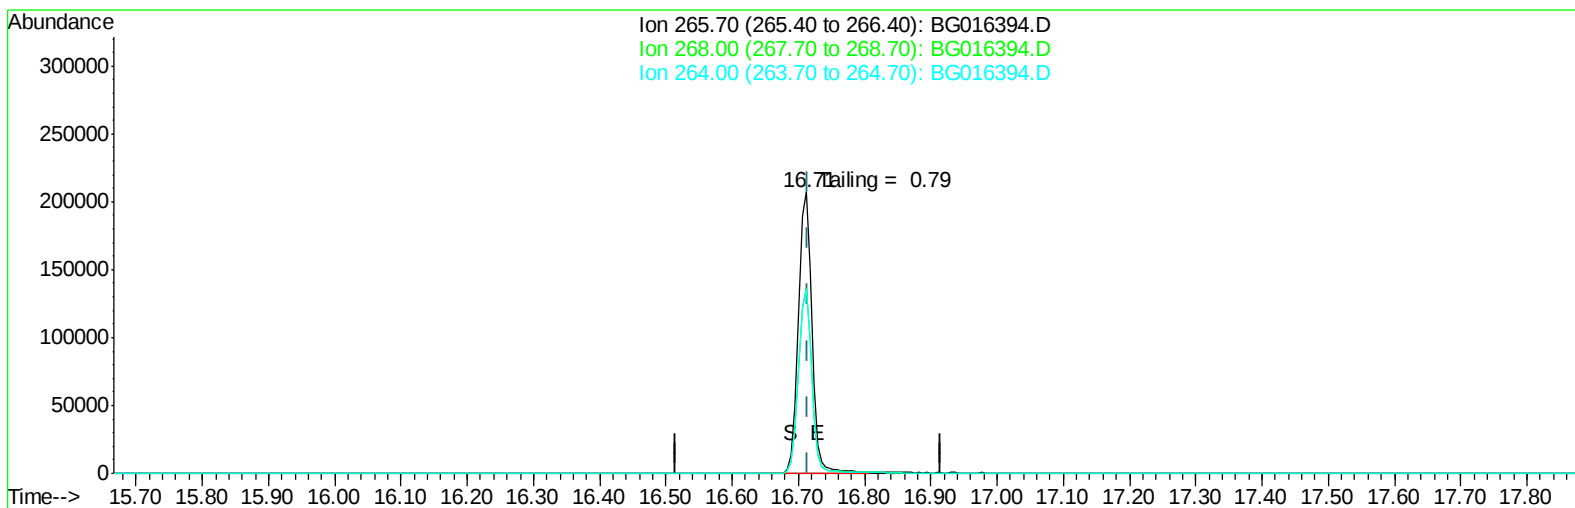

TIC: BG016394.D

(69) Pentachlorophenol (C)



16.712min (-0.004) 33621.84ng

response 304278

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	65.74
264.00	66.00	65.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041415\
 Data File : BG016394.D
 Acq On : 14 Apr 2015 13:45
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 06:57:32 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 14 14:00:56 2015
 Response via : Initial Calibration

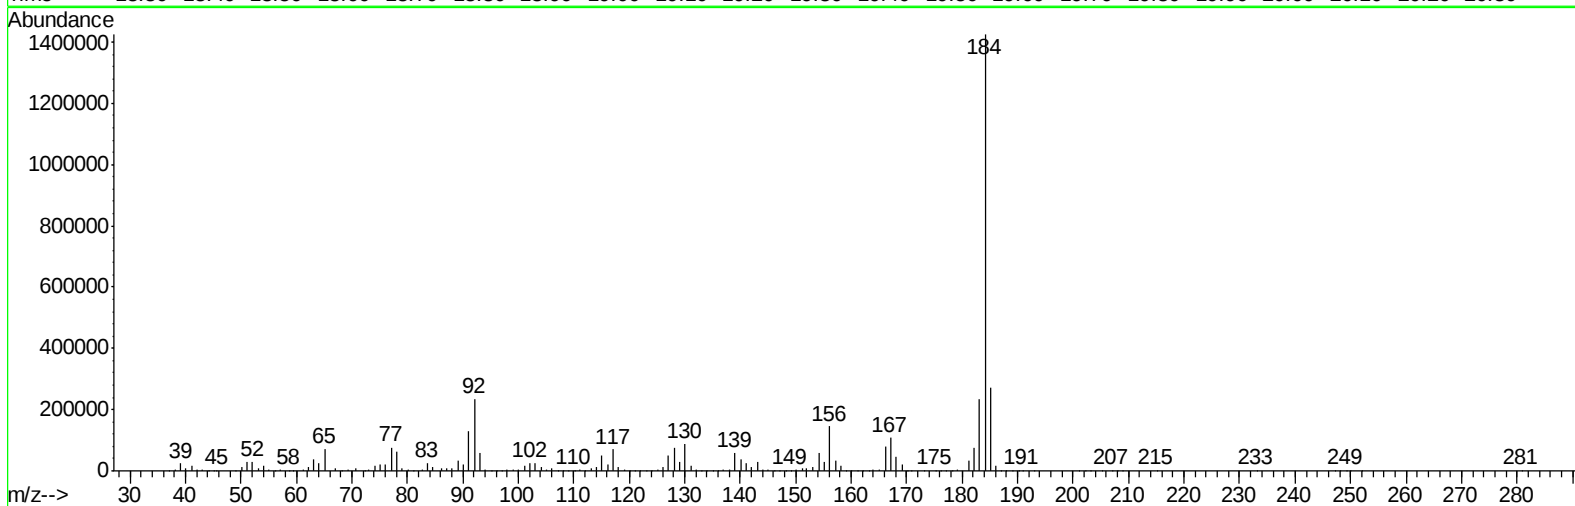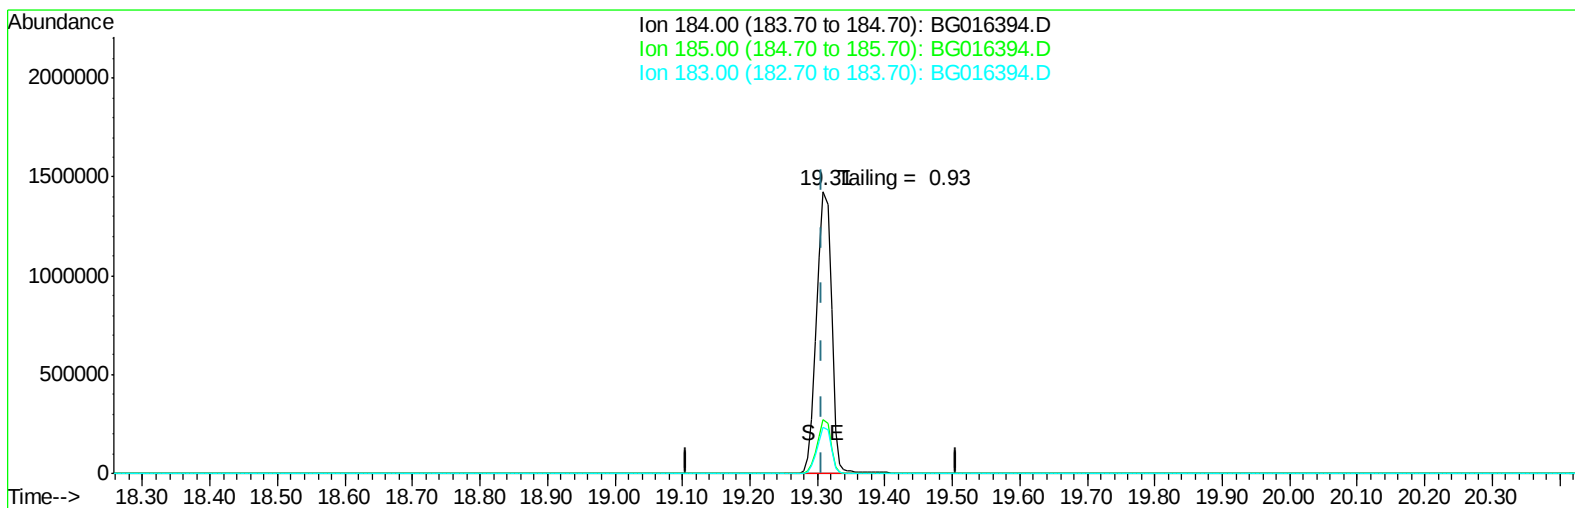

TIC: BG016394.D

(76) Benzidine

19.309min (+0.002) 15537.12ng

response 2155224

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	19.12#
183.00	13.00	16.46#
0.00	0.00	0.00