

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041416\
 Data File : BG021665.D
 Acq On : 14 Apr 2016 23:13
 Operator : UM/SJ
 Sample : H2517-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 S8-0569

Quant Time: Apr 15 00:56:32 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 15:48:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.22	152	29271	20.00	ng	0.00
21) Naphthalene-d8	11.03	136	137265	20.00	ng	0.00
38) Acenaphthene-d10	14.82	164	94348	20.00	ng	0.00
63) Phenanthrene-d10	17.56	188	217872	20.00	ng	0.00
75) Chrysene-d12	21.83	240	238753	20.00	ng	0.00
86) Perylene-d12	25.15	264	234330	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.76	112	128077	72.86	ng	0.00
7) Phenol-d6	7.36	99	119784	45.62	ng	0.00
23) Nitrobenzene-d5	9.38	82	275525	103.17	ng	0.00
41) 2,4,6-Tribromophenol	16.30	330	183961	180.92	ng	0.00
44) 2-Fluorobiphenyl	13.45	172	646684	100.43	ng	0.00
78) Terphenyl-d14	20.15	244	924231	96.59	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.54	79	4308	2.15	ng	Qvalue # 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041416\
Data File : BG021665.D
Acq On : 14 Apr 2016 23:13
Operator : UM/SJ
Sample : H2517-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S8-0569

Quant Time: Apr 15 00:56:32 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

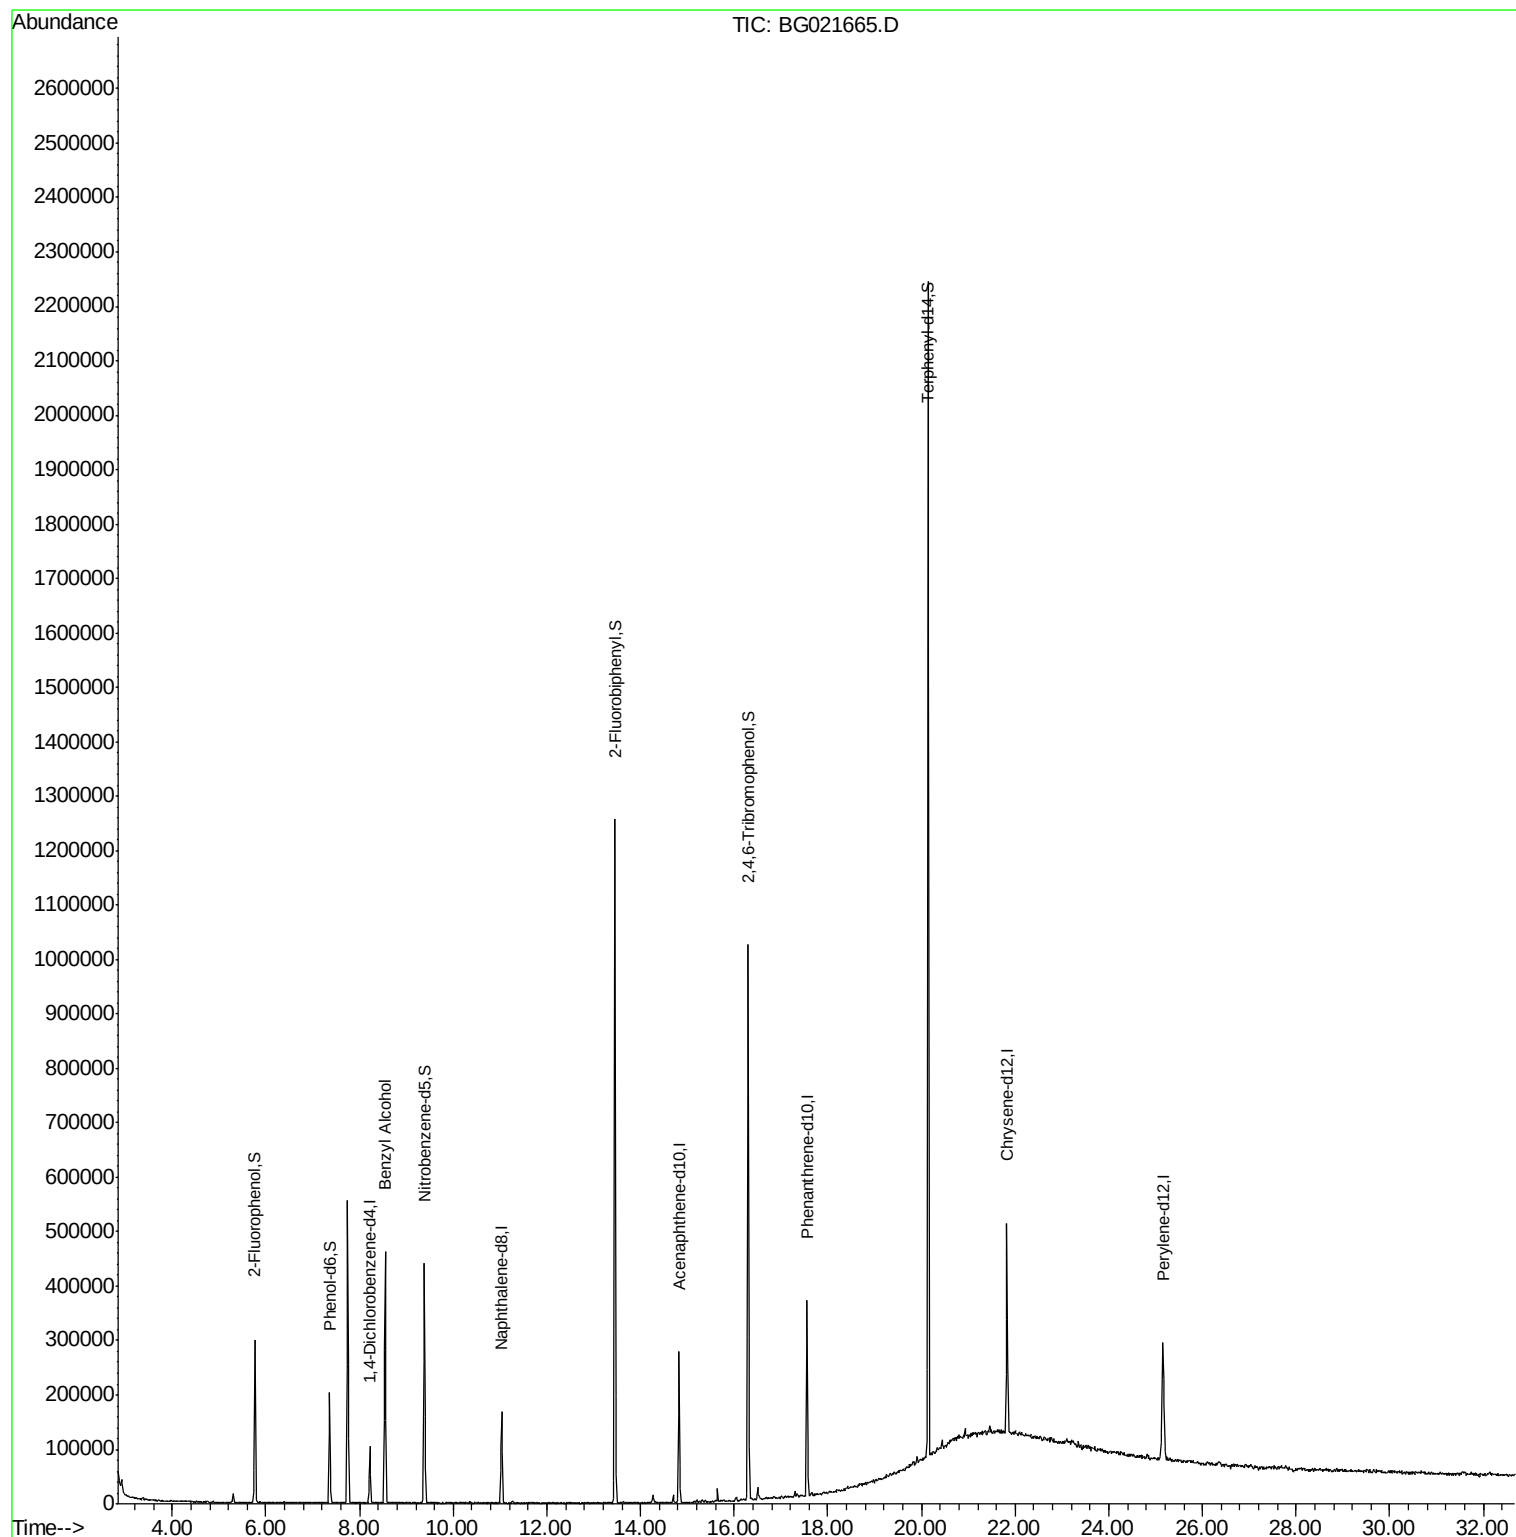

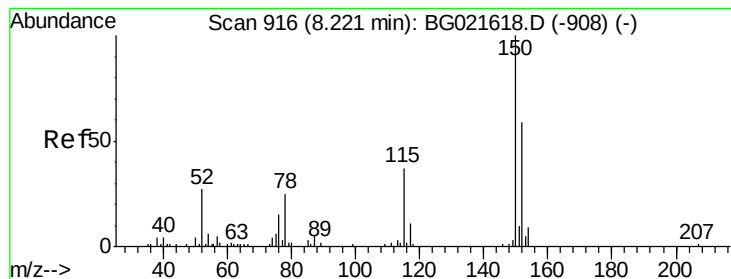

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.22 min Scan# 916

Delta R.T. -0.00 min

Lab File: BG021665.D

Acq: 14 Apr 2016 23:13

Instrument :

BNA_G

ClientSampleId :

S8-0569


Tgt Ion:152 Resp: 29271

Ion Ratio Lower Upper

152 100

150 153.4 130.1 195.1




115 61.7 62.2 93.2#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

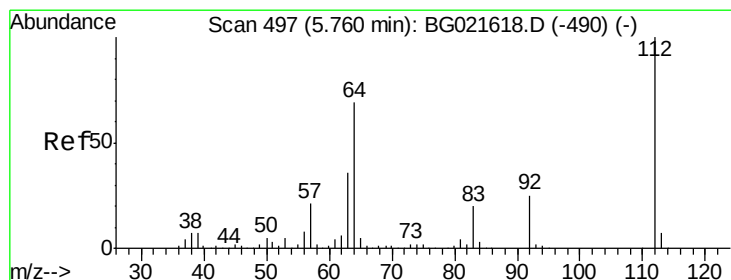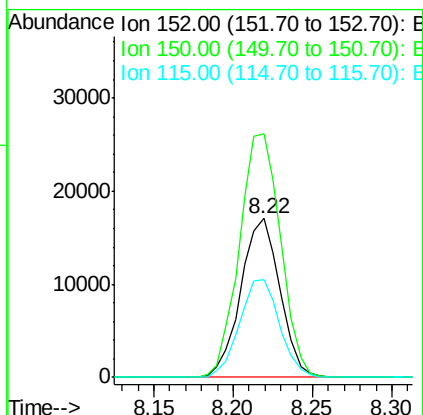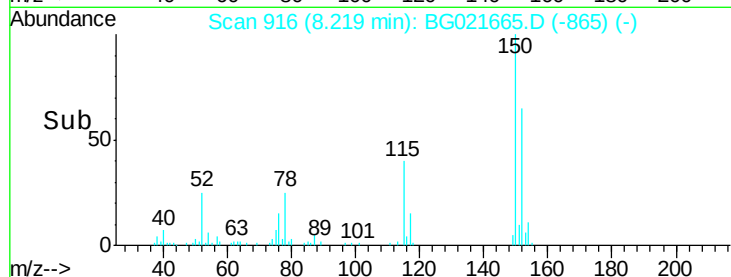

#5

2-Fluorophenol

Concen: 72.86 ng

RT: 5.76 min Scan# 498

Delta R.T. 0.00 min

Lab File: BG021665.D

Acq: 14 Apr 2016 23:13


Tgt Ion:112 Resp: 128077

Ion Ratio Lower Upper

112 100

64 69.8 51.1 76.7



63 35.7 24.6 37.0




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

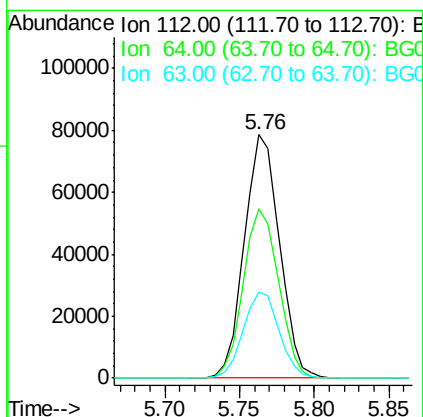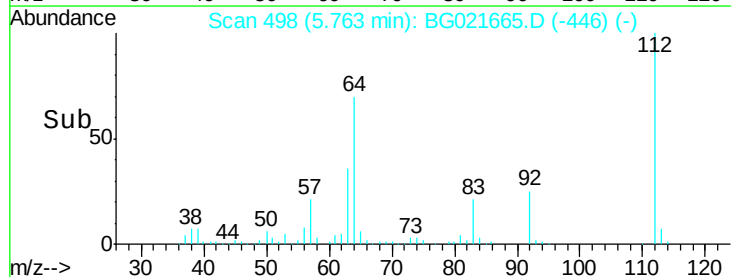

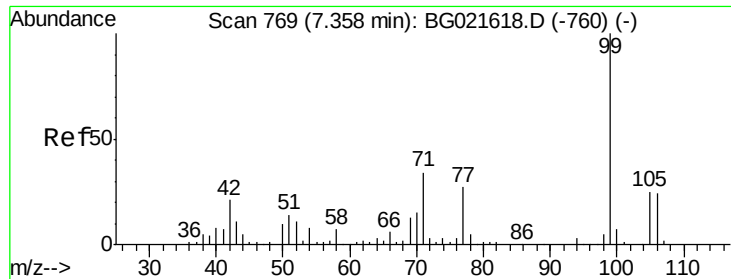

#7

Phenol-d6

Concen: 45.62 ng

RT: 7.36 min Scan# 770

Delta R.T. 0.00 min

Lab File: BG021665.D

Acq: 14 Apr 2016 23:13

Instrument :

BNA_G

ClientSampleId :

S8-0569


Tgt Ion: 99 Resp: 119784

Ion Ratio Lower Upper




99 100

42 20.1 16.4 24.6

71 33.8 25.0 37.4

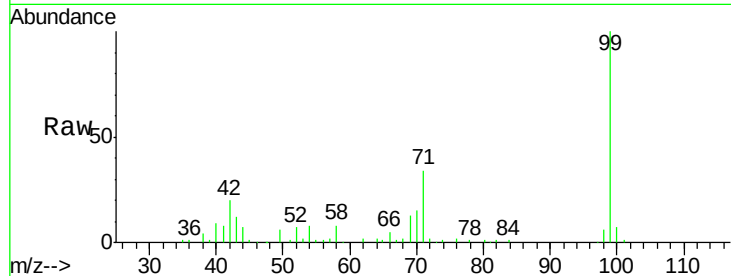

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

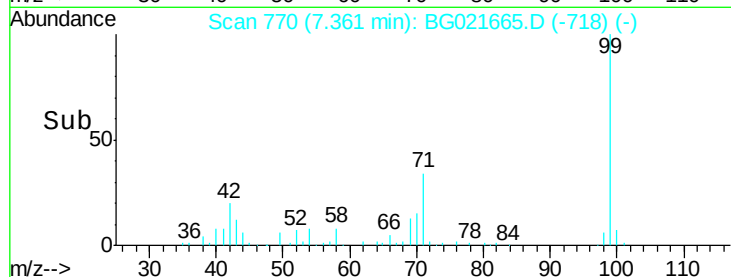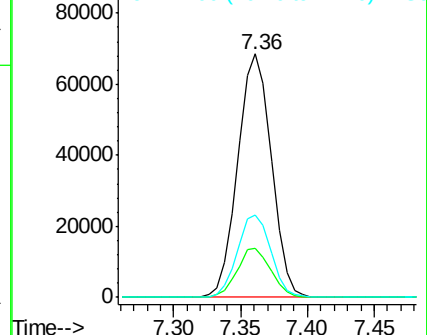

#15

Benzyl Alcohol

Concen: 2.15 ng

RT: 8.54 min Scan# 971

Delta R.T. 0.09 min

Lab File: BG021665.D

Acq: 14 Apr 2016 23:13


Tgt Ion: 79 Resp: 4308

Ion Ratio Lower Upper



79 100


108 30.9 59.4 89.0#

77 82.4 52.2 78.2#



Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC

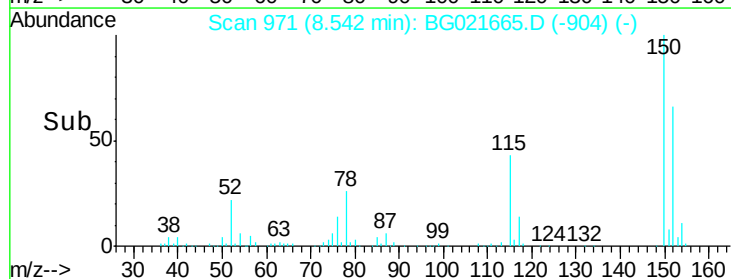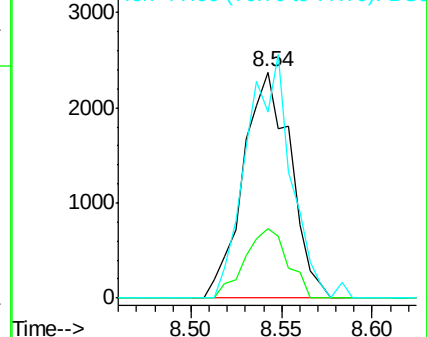


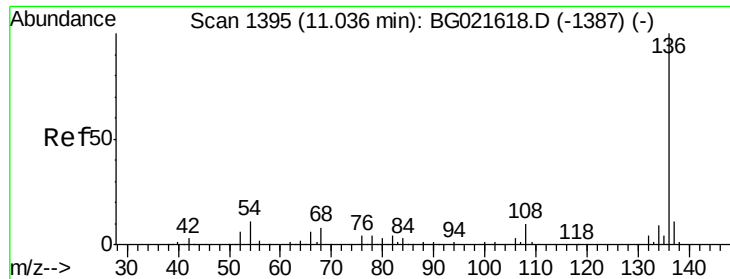




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.03 min Scan# 1395
Delta R.T. -0.00 min
Lab File: BG021665.D
Acq: 14 Apr 2016 23:13

Instrument :
BNA_G
ClientSampleId :
S8-0569

Tgt Ion:	136	Resp:	137265
Ion	Ratio	Lower	Upper
136	100		
137	10.9	9.0	13.4
54	11.1	9.6	14.4
68	6.7	6.4	9.6

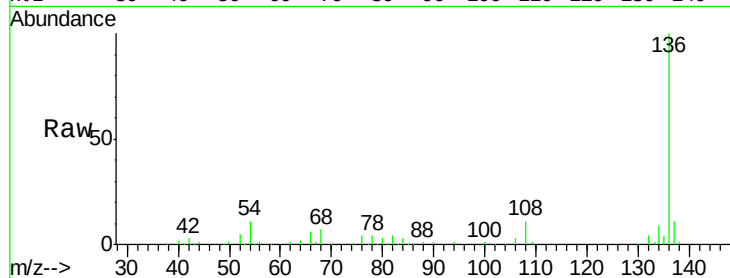


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

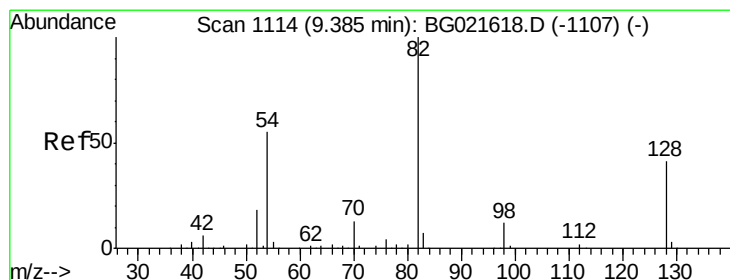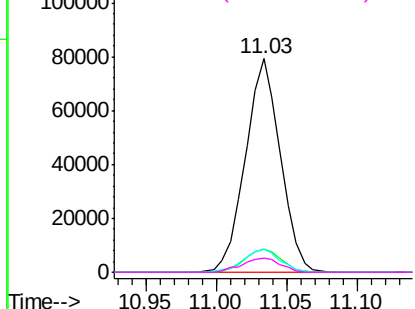
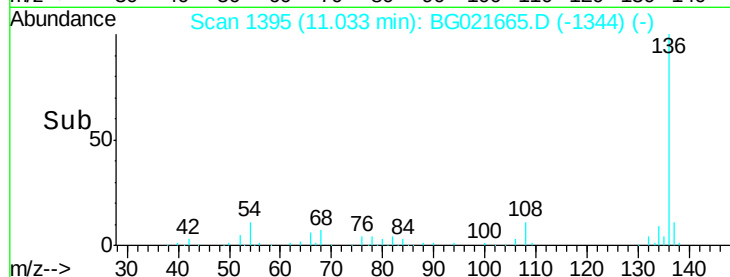



#23
Nitrobenzene-d5
Concen: 103.17 ng
RT: 9.38 min Scan# 1114
Delta R.T. -0.00 min
Lab File: BG021665.D
Acq: 14 Apr 2016 23:13

Tgt Ion:	82	Resp:	275525
Ion	Ratio	Lower	Upper
82	100		
128	40.6	33.4	50.0
54	52.4	46.1	69.1

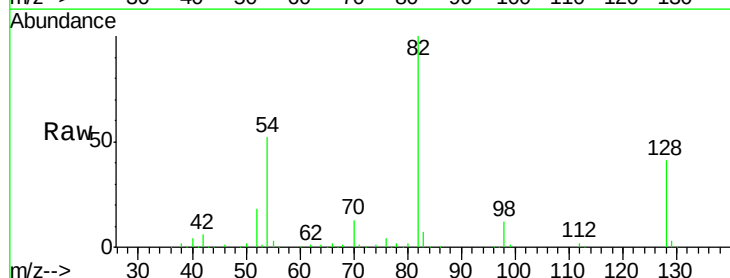

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

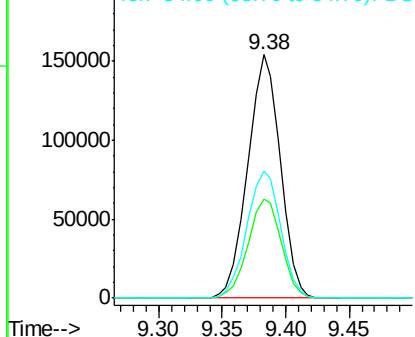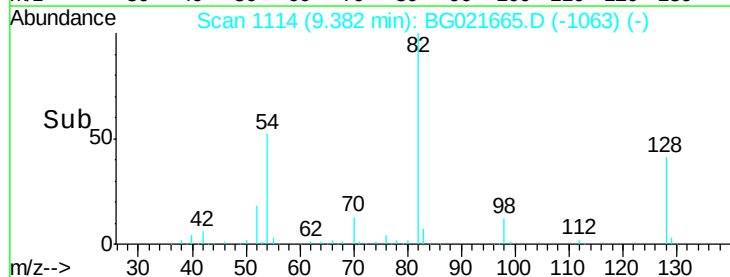

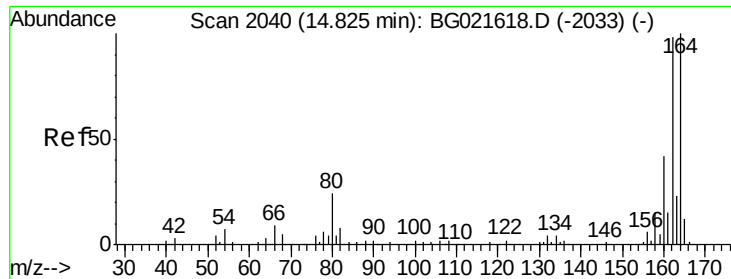

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.82 min Scan# 2040

Delta R.T. -0.00 min

Lab File: BG021665.D

Acq: 14 Apr 2016 23:13

Instrument :

BNA_G

ClientSampleId :

S8-0569


Tgt Ion:164 Resp: 94348

Ion Ratio Lower Upper

164 100

162 104.4 78.0 117.0




160 42.6 32.9 49.3

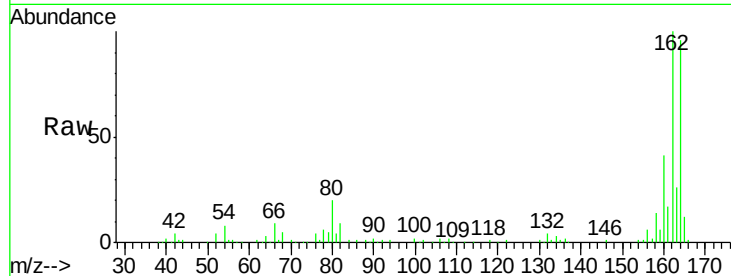

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

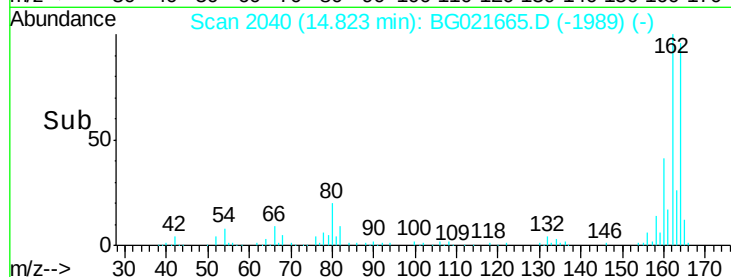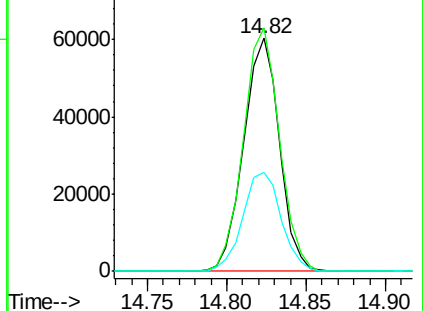

#41

2,4,6-Tribromophenol

Concen: 180.92 ng

RT: 16.30 min Scan# 2292

Delta R.T. -0.00 min

Lab File: BG021665.D

Acq: 14 Apr 2016 23:13


Tgt Ion:330 Resp: 183961

Ion Ratio Lower Upper

330 100

332 96.1 78.0 117.0



141 40.3 33.8 50.8




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



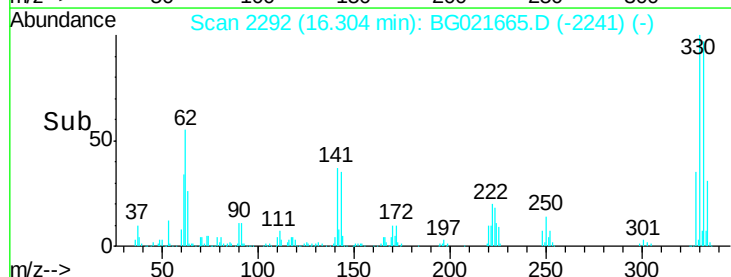
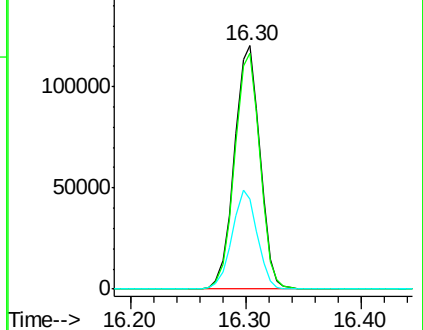


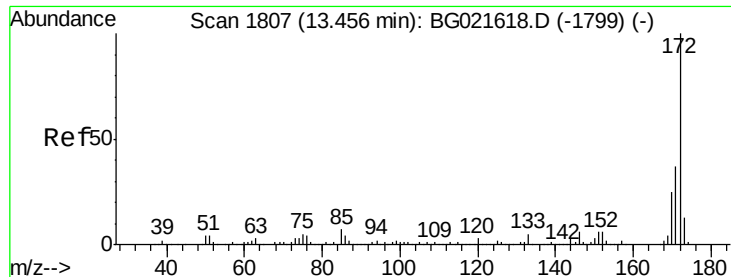

#44
 2-Fluorobiphenyl
 Concen: 100.43 ng
 RT: 13.45 min Scan# 1807
 Delta R.T. -0.00 min
 Lab File: BG021665.D
 Acq: 14 Apr 2016 23:13




Instrument :
 BNA_G
 ClientSampled :
 S8-0569


Tgt Ion:172 Resp: 646684
 Ion Ratio Lower Upper
 172 100
 171 39.8 27.8 41.6
 170 24.9 19.6 29.4

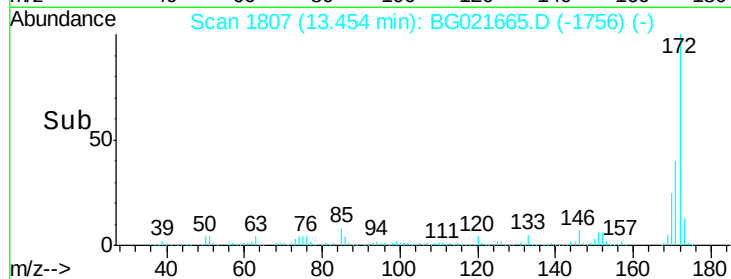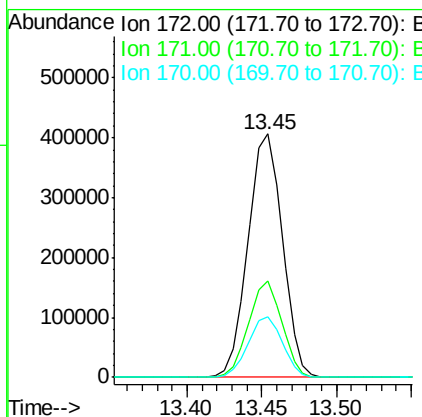

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 17.56 min Scan# 2505
 Delta R.T. -0.01 min
 Lab File: BG021665.D
 Acq: 14 Apr 2016 23:13

Tgt Ion:188 Resp: 217872
 Ion Ratio Lower Upper
 188 100
 94 9.0 7.5 11.3
 80 10.4 8.6 13.0

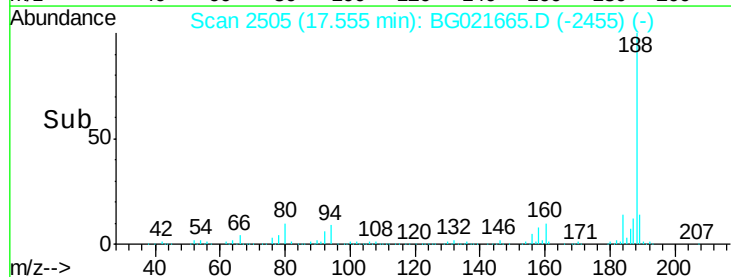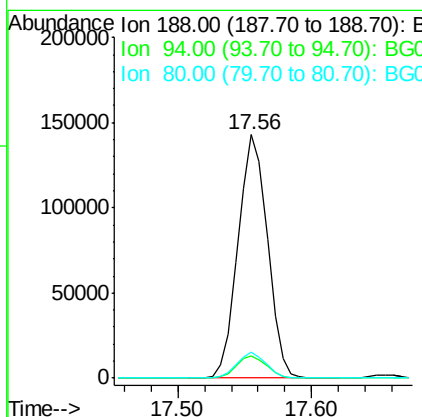

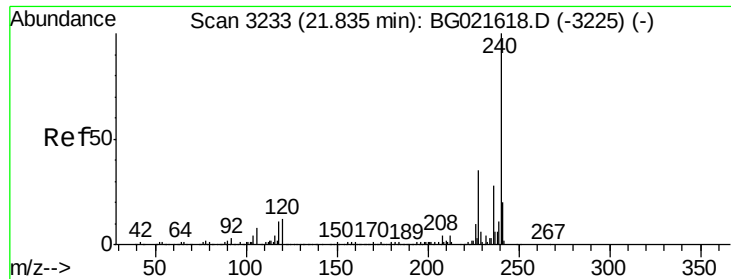

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.83 min Scan# 3232

Delta R.T. -0.01 min

Lab File: BG021665.D

Acq: 14 Apr 2016 23:13

Instrument :

BNA_G

ClientSampleId :

S8-0569


Tgt Ion:240 Resp: 238753

Ion Ratio Lower Upper

240 100

120 11.6 8.4 12.6




236 27.7 19.6 29.4



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

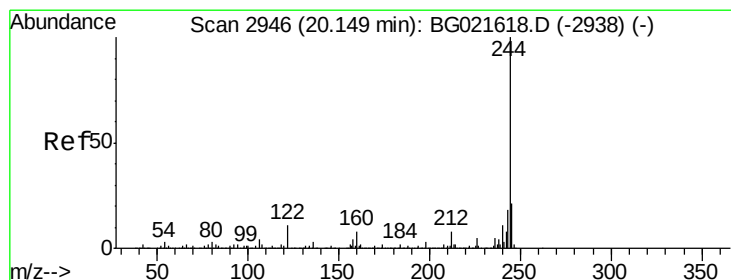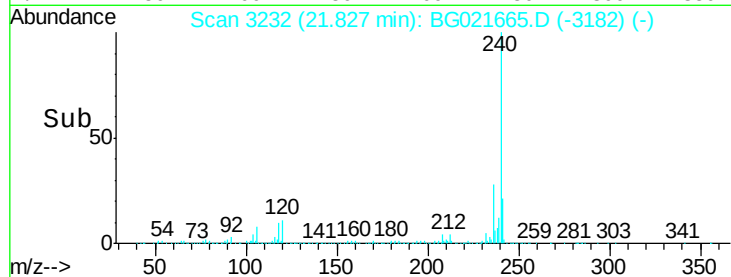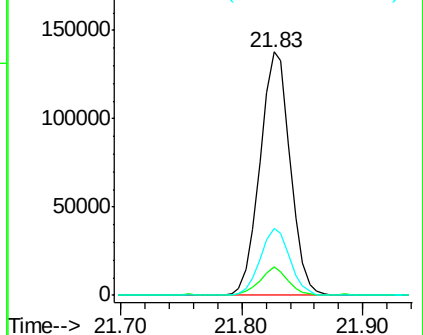

#78

Terphenyl-d14

Concen: 96.59 ng

RT: 20.15 min Scan# 2946

Delta R.T. -0.00 min

Lab File: BG021665.D

Acq: 14 Apr 2016 23:13


Tgt Ion:244 Resp: 924231

Ion Ratio Lower Upper

244 100

212 8.6 6.5 9.7



122 10.8 8.6 12.8






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

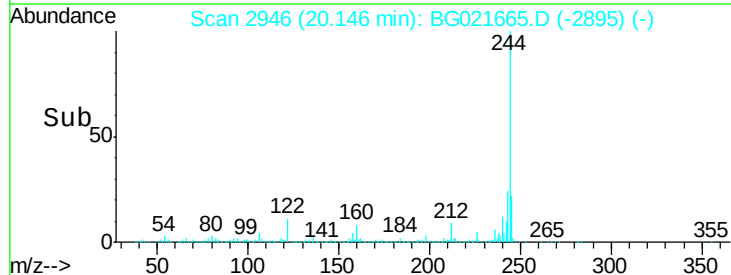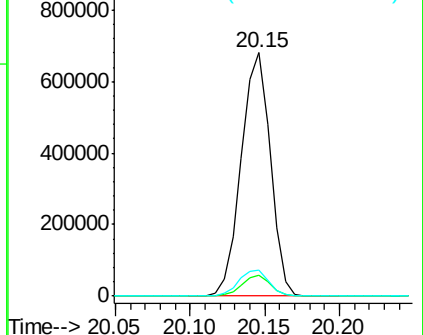

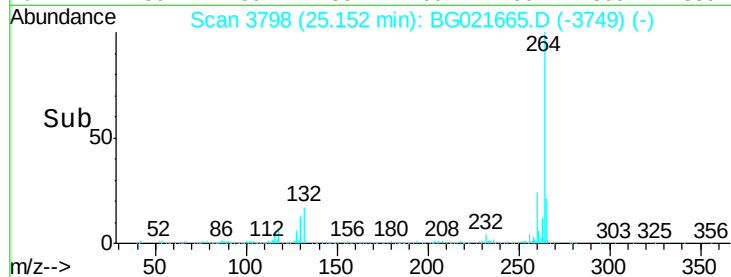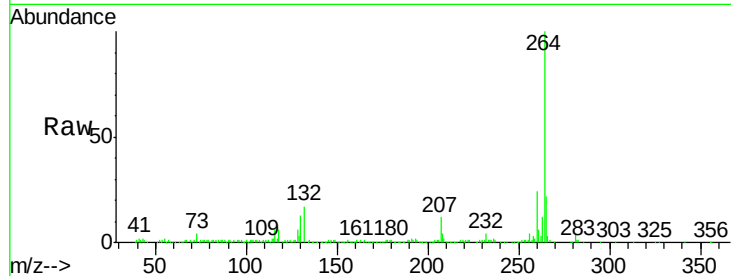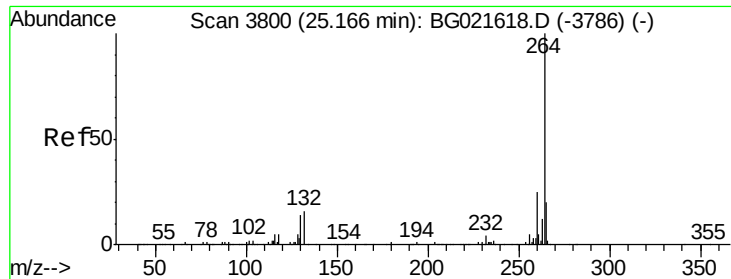

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.15 min Scan# 3798

Delta R.T. -0.01 min

Lab File: BG021665.D

Acq: 14 Apr 2016 23:13

Instrument :

BNA_G

ClientSampleId :

S8-0569

Tgt Ion: 264 Resp: 234330

Ion Ratio Lower Upper

264 100

260 23.8 20.2 30.4

265 21.6 17.8 26.8

