
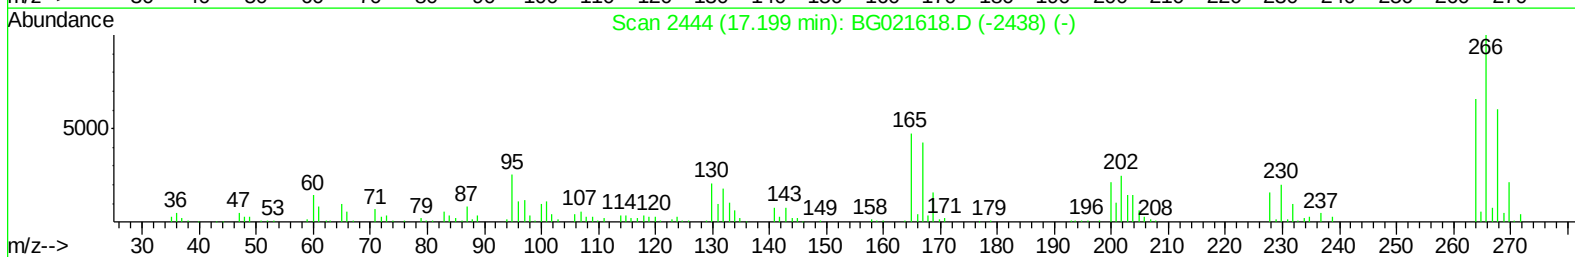
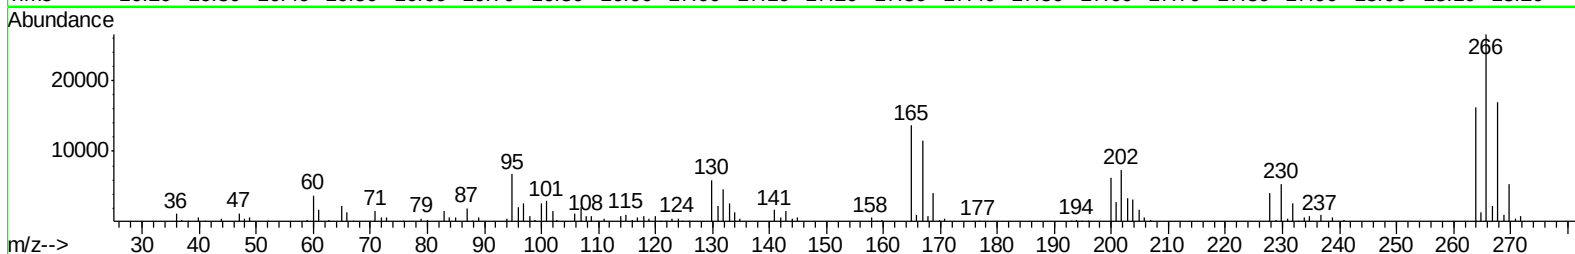


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041416\
Data File : BG021659.D
Acq On : 14 Apr 2016 19:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 05:56:57 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

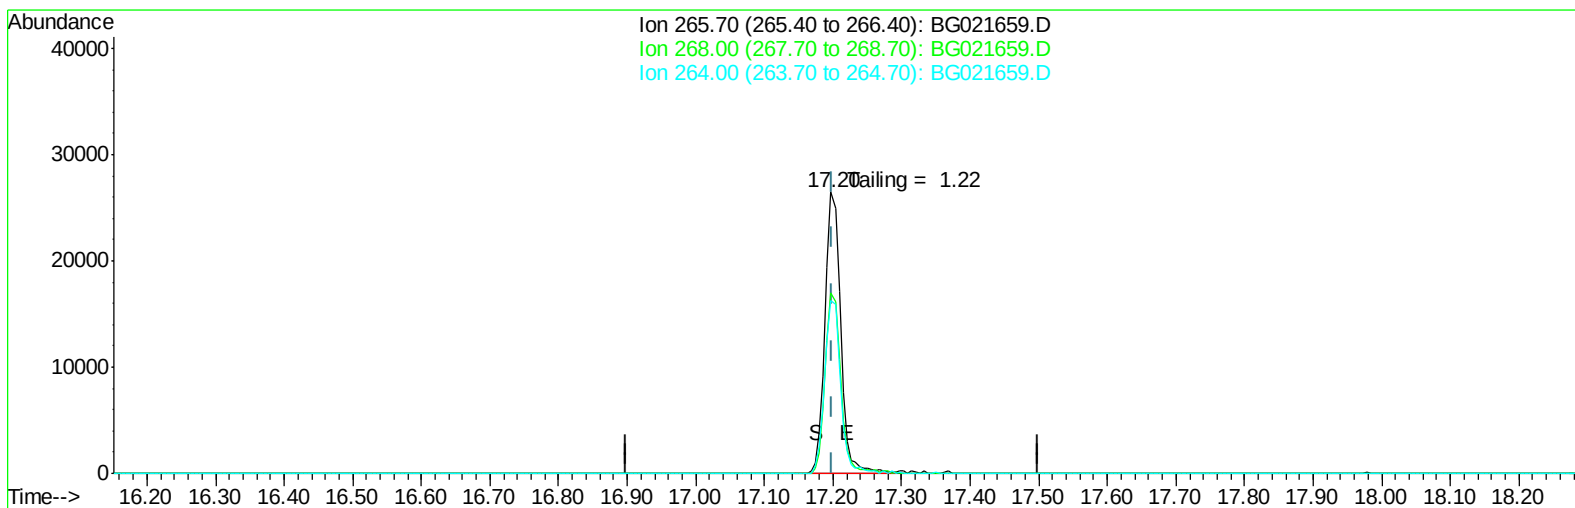

TIC: BG021659.D

(69) Pentachlorophenol (C)




17.198min (-0.002) 0.00ng

response 41723

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	64.24
264.00	67.20	61.36
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041416\
Data File : BG021659.D
Acq On : 14 Apr 2016 19:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 05:56:57 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

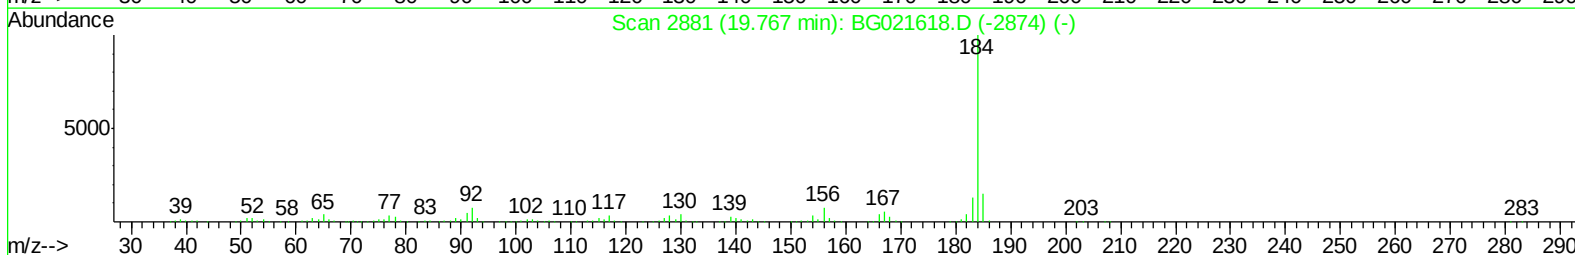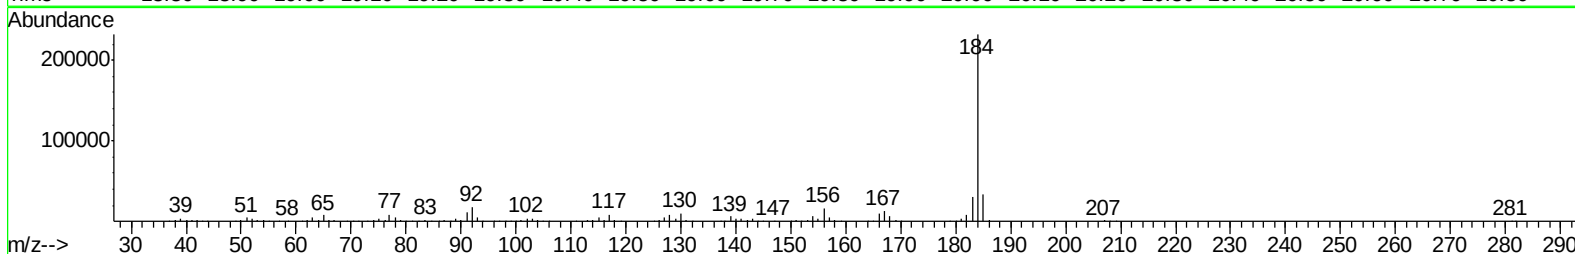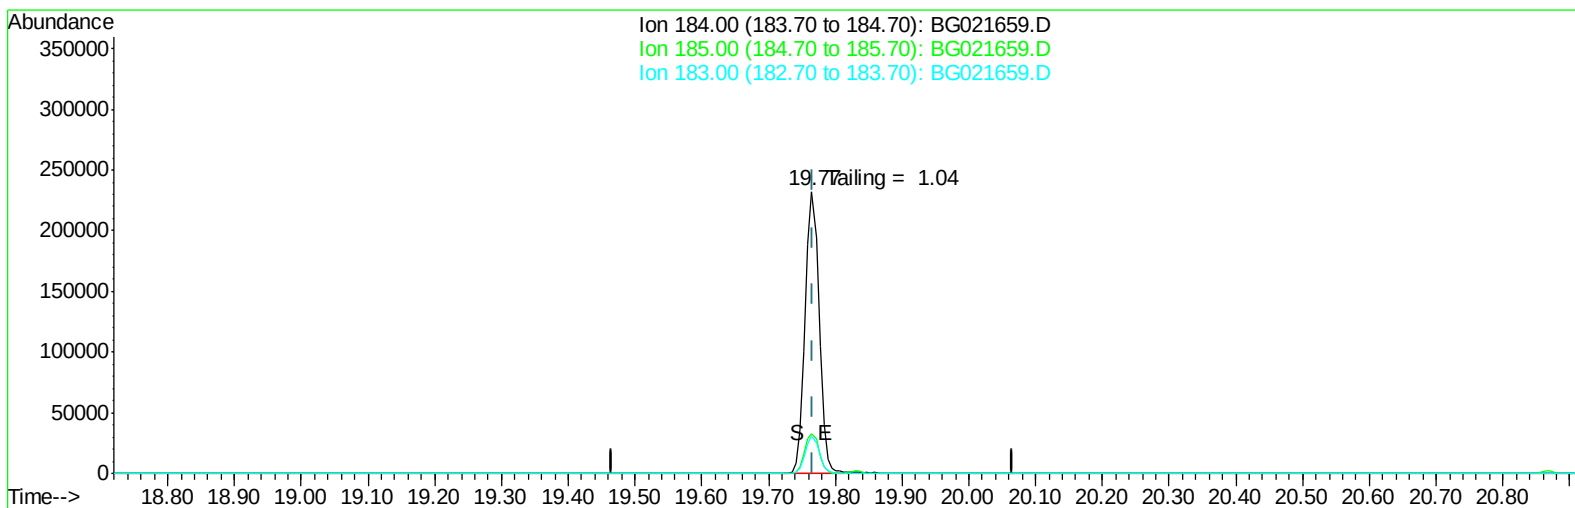

TIC: BG021659.D

(76) Benzidine

19.765min (-0.002) 200141.48ng

response 330269

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.27
183.00	12.80	13.38
0.00	0.00	0.00