


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041416\
 Data File : BG021644.D
 Acq On : 14 Apr 2016 8:14
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 15:48:13 2016

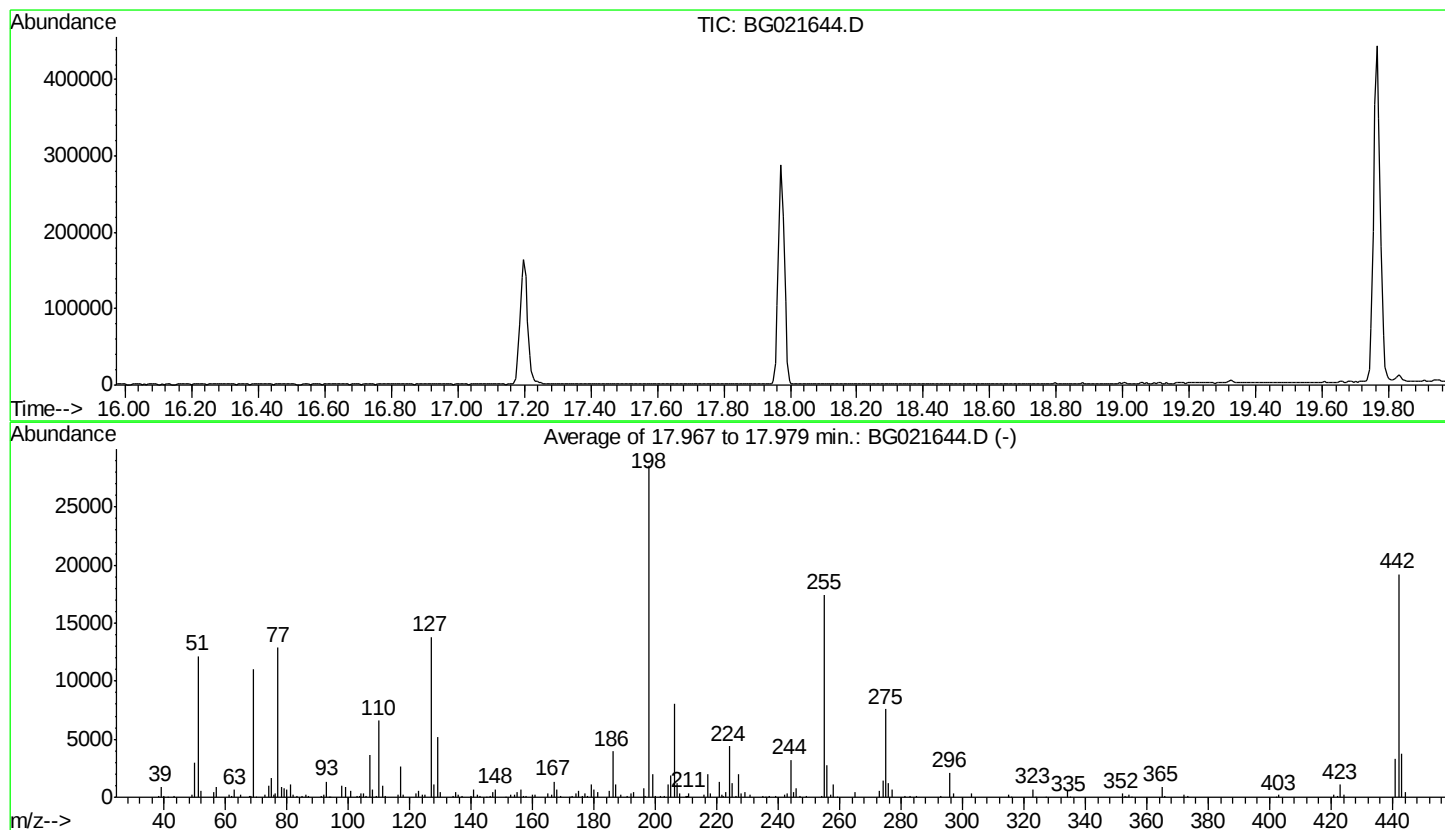

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	12168	PASS
68	69	0.00	2	1.2	134	PASS
69	198	0.00	100	38.4	10980	PASS
70	69	0.00	2	0.5	58	PASS
127	198	10	80	48.4	13826	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28565	PASS
199	198	5	9	6.9	1961	PASS
275	198	10	60	26.5	7569	PASS
365	198	1	100	3.2	915	PASS
441	442	0.01	24	17.2	3304	PASS
442	198	50	100	67.3	19216	PASS
443	442	15	24	19.3	3703	PASS