


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041416\
Data File : BG021659.D
Acq On : 14 Apr 2016 19:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 13 15:48:13 2016

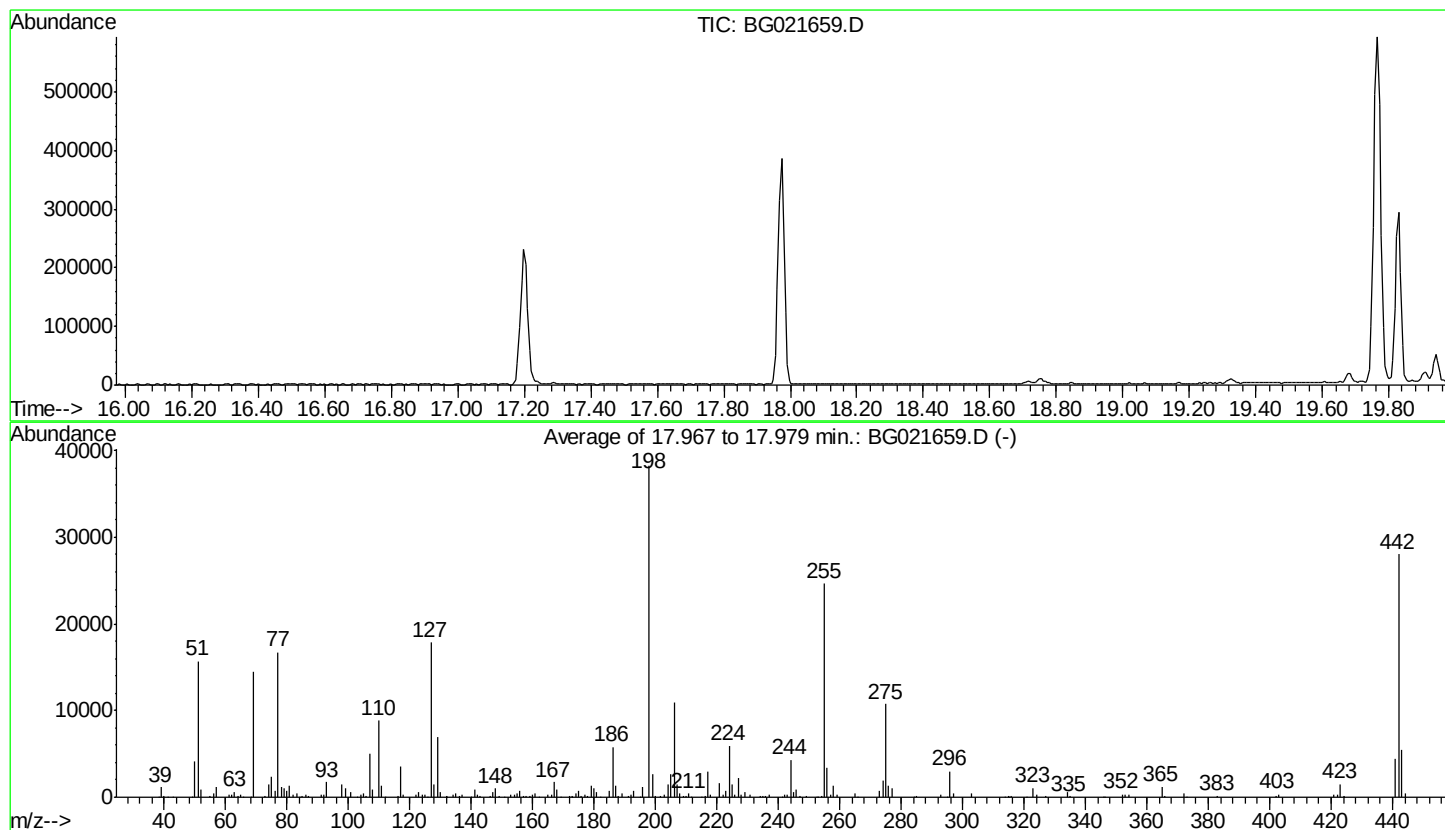

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	15670	PASS
68	69	0.00	2	0.5	71	PASS
69	198	0.00	100	38.0	14537	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	17846	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38261	PASS
199	198	5	9	6.9	2649	PASS
275	198	10	60	28.1	10735	PASS
365	198	1	100	3.3	1258	PASS
441	442	0.01	24	16.0	4483	PASS
442	198	50	100	73.3	28053	PASS
443	442	15	24	19.4	5456	PASS