
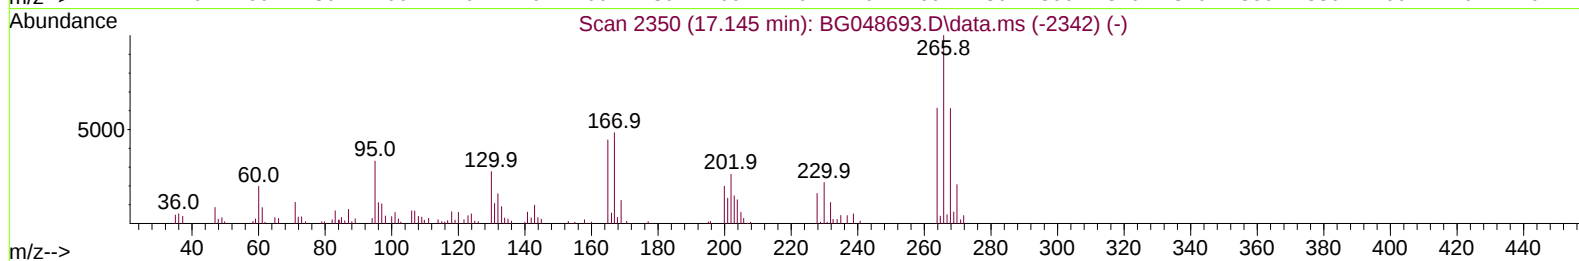
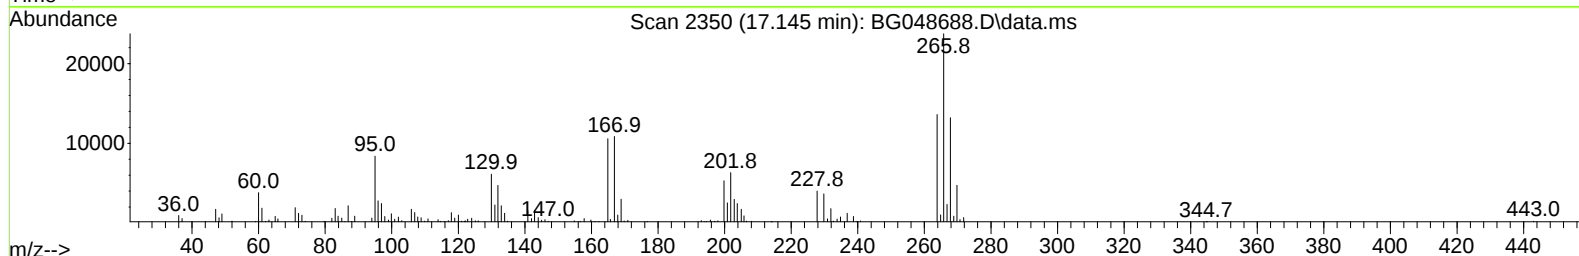


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041421\
Data File : BG048688.D
Acq On : 14 Apr 2021 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 10:02:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 15 01:59:11 2021
Response via : Initial Calibration

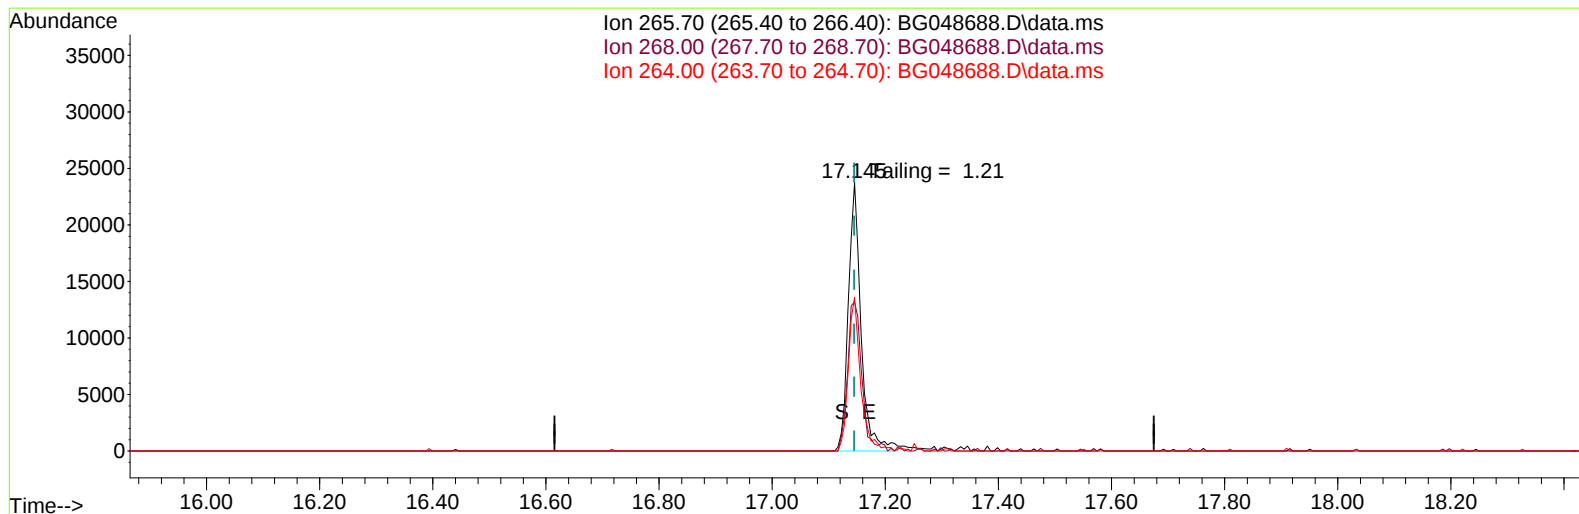

TIC: BG048688.D\data.ms

(70) Pentachlorophenol (C)




17.145min (+ 0.000) 10574.58 ng

response 38167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	55.60
264.00	61.30	57.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041421\
Data File : BG048688.D
Acq On : 14 Apr 2021 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 10:02:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 15 01:59:11 2021
Response via : Initial Calibration

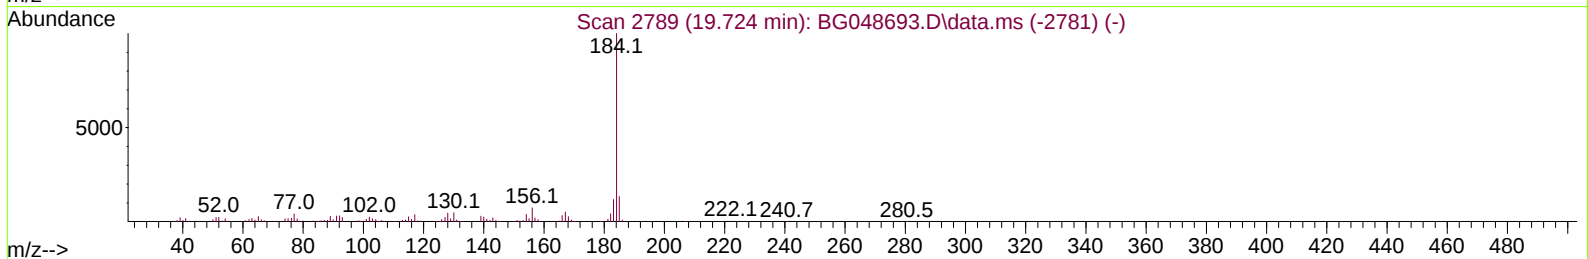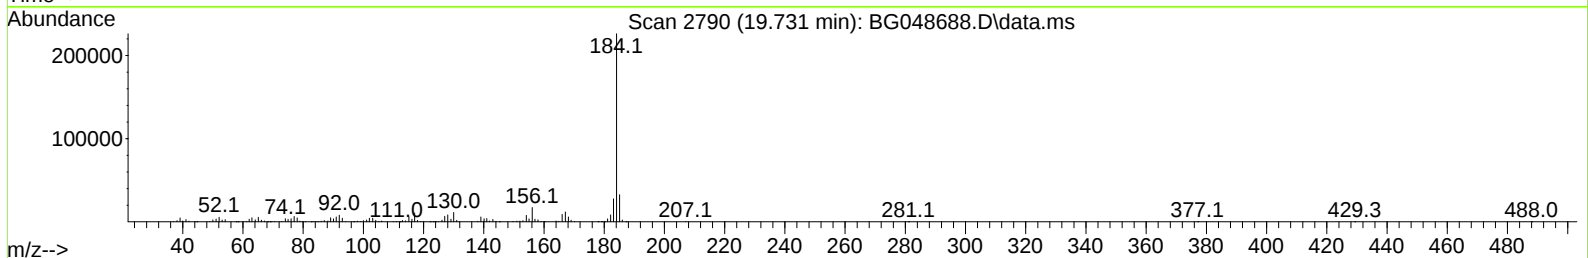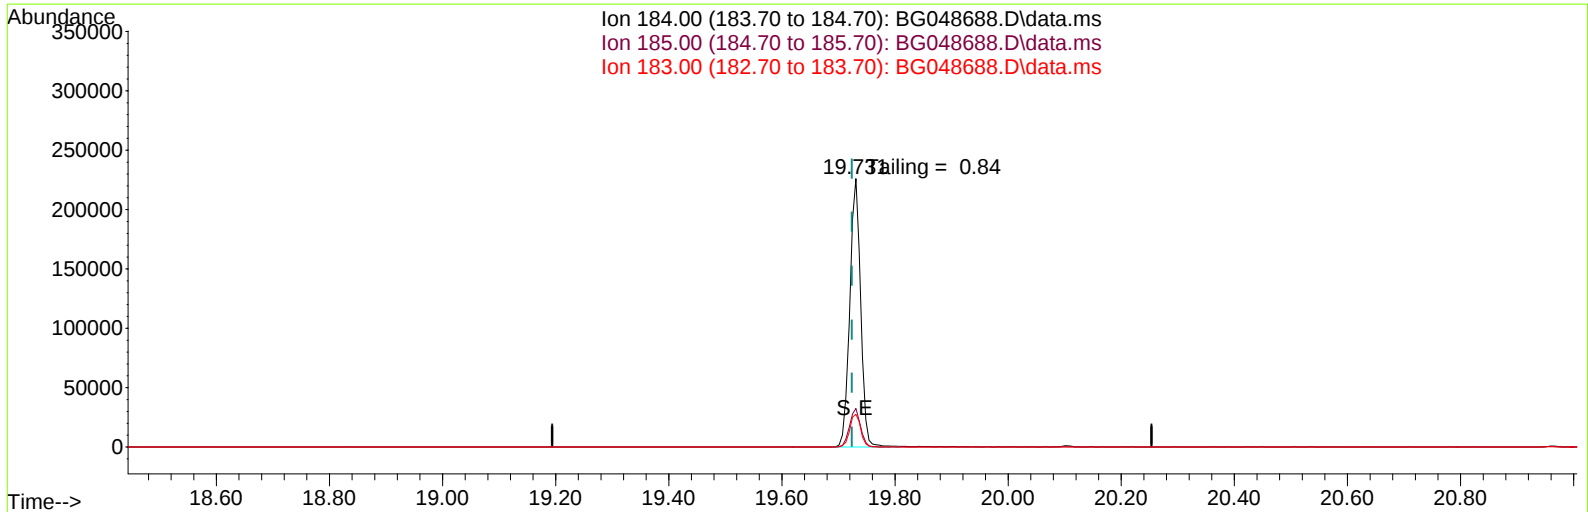

TIC: BG048688.D\data.ms

(77) Benzidine**19.731min (+ 0.007) 206428.49 ng****response 302715**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.41
183.00	11.70	12.20
0.00	0.00	0.00