


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041421\
 Data File : BG048688.D
 Acq On : 14 Apr 2021 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 15 10:59:37 2021

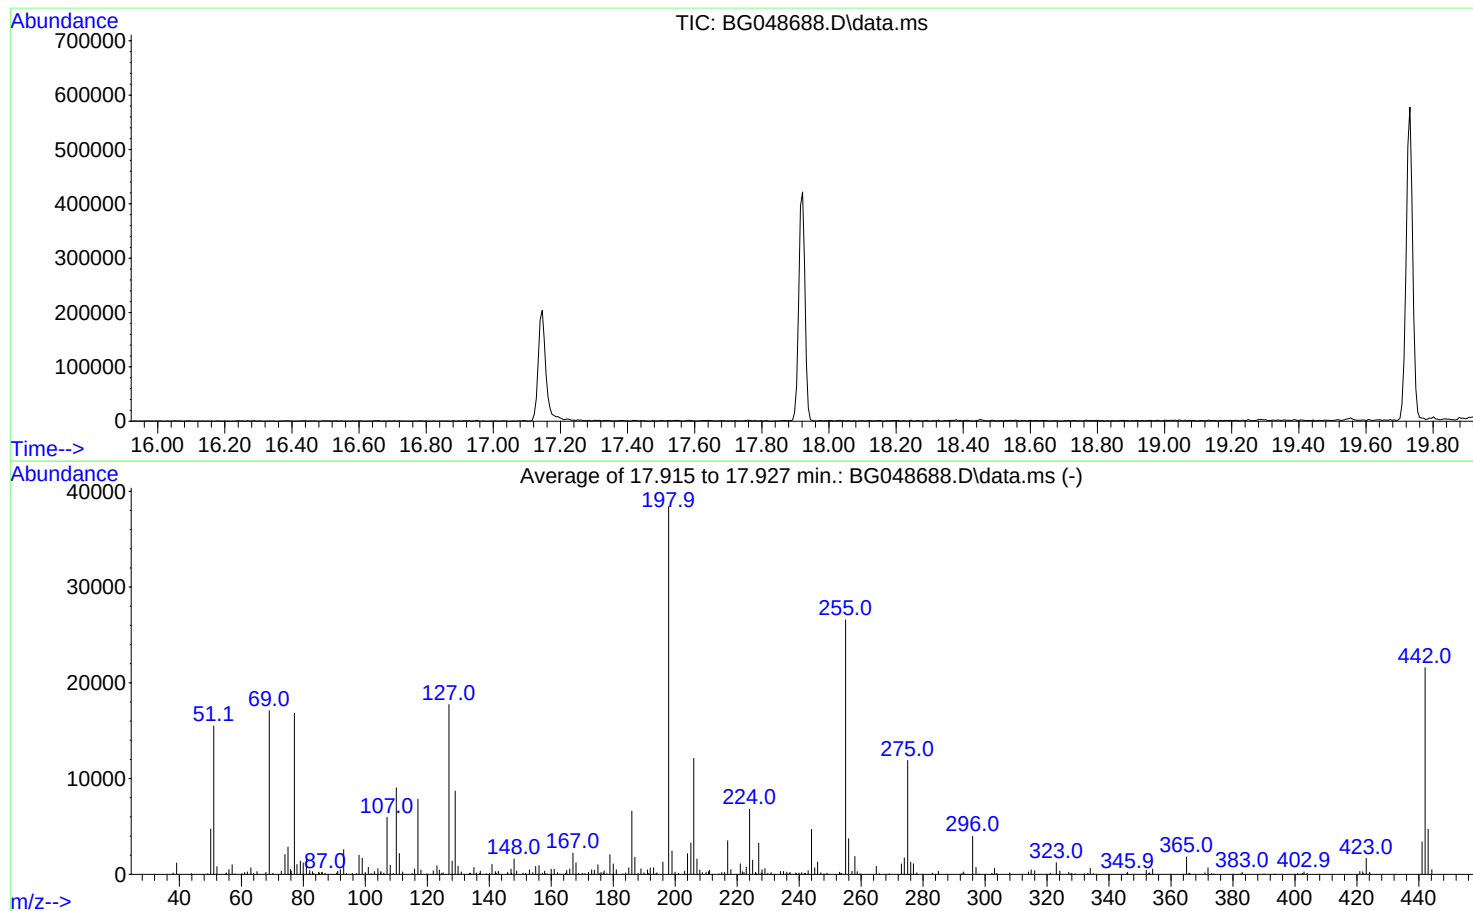




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	15489	PASS
68	69	0.00	2	1.3	221	PASS
69	198	0.00	100	44.5	17096	PASS
70	69	0.00	2	0.6	103	PASS
127	198	10	80	46.2	17732	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38408	PASS
199	198	5	9	6.4	2439	PASS
275	198	10	60	31.0	11892	PASS
365	198	1	100	4.7	1814	PASS
441	198	0.01	100	8.8	3399	PASS
442	198	50	100	56.2	21589	PASS
443	442	15	24	21.8	4711	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041421\
 Data File : BG048688.D
 Acq On : 14 Apr 2021 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 15 10:02:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 15 01:59:11 2021
 Response via : Initial Calibration

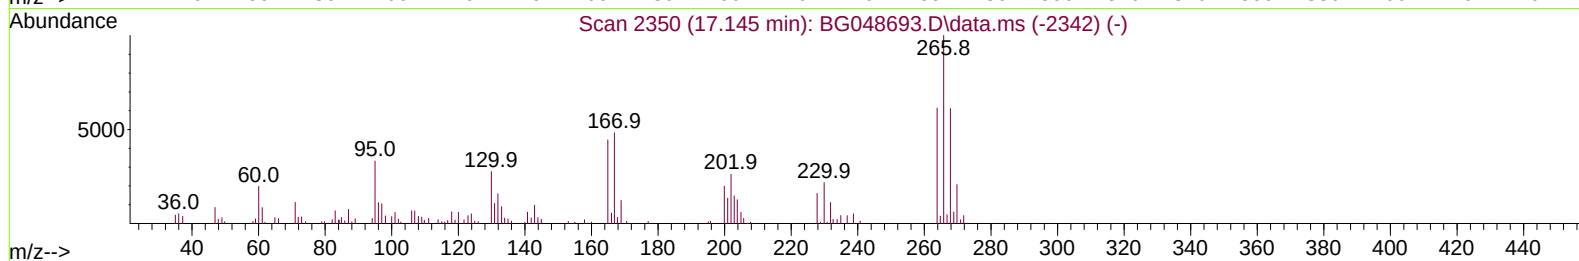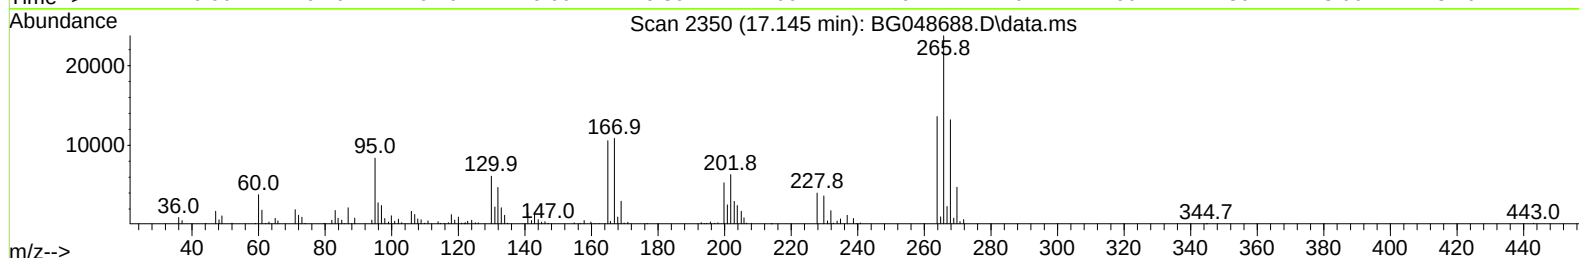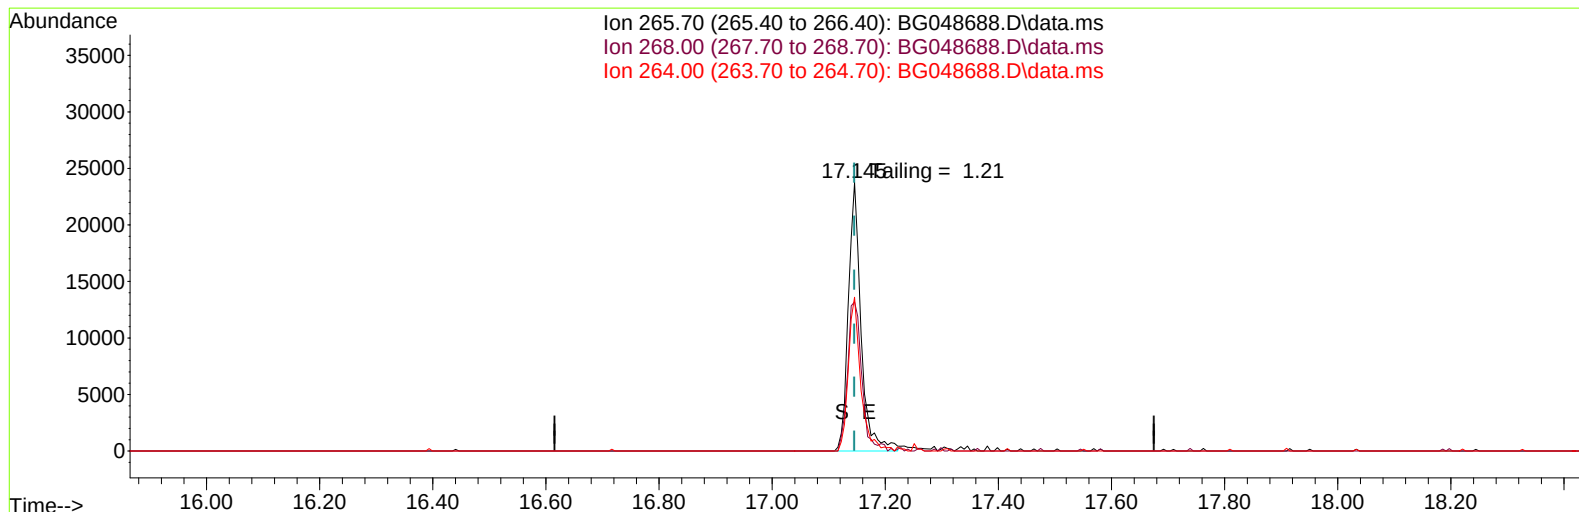

TIC: BG048688.D\data.ms

(70) Pentachlorophenol (C)

17.145min (+ 0.000) 10574.58 ng




response 38167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	55.60
264.00	61.30	57.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041421\
Data File : BG048688.D
Acq On : 14 Apr 2021 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 15 10:02:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 15 01:59:11 2021
Response via : Initial Calibration

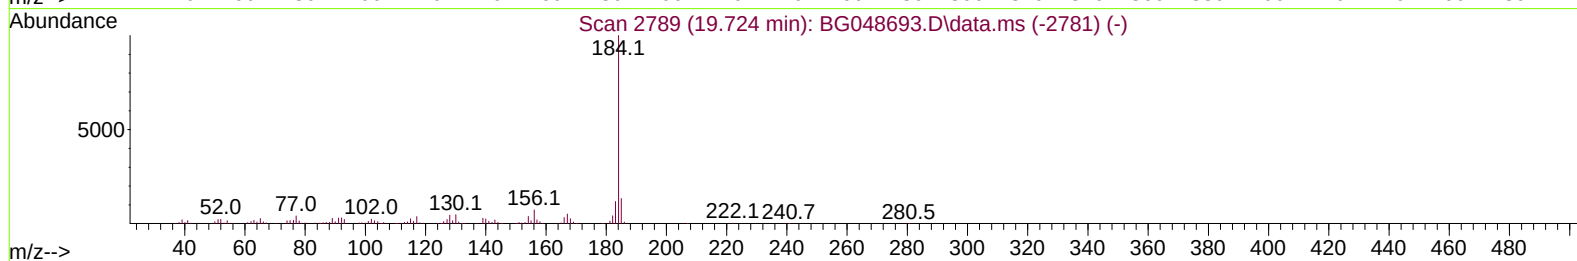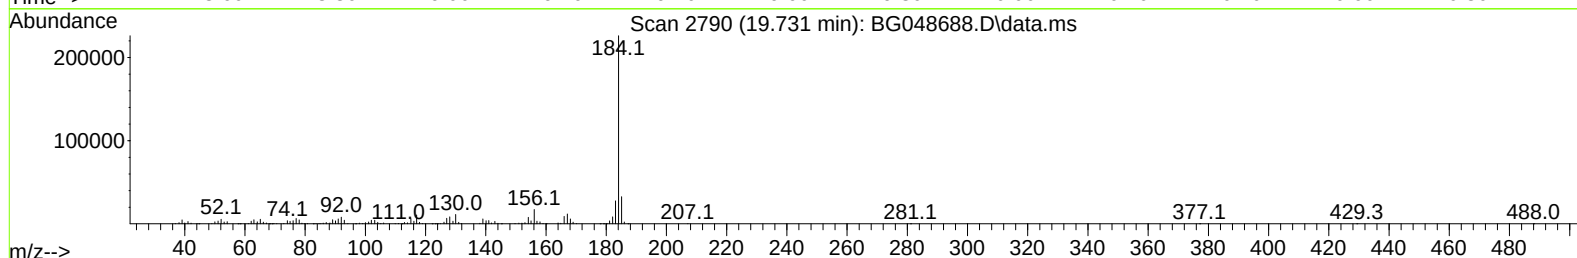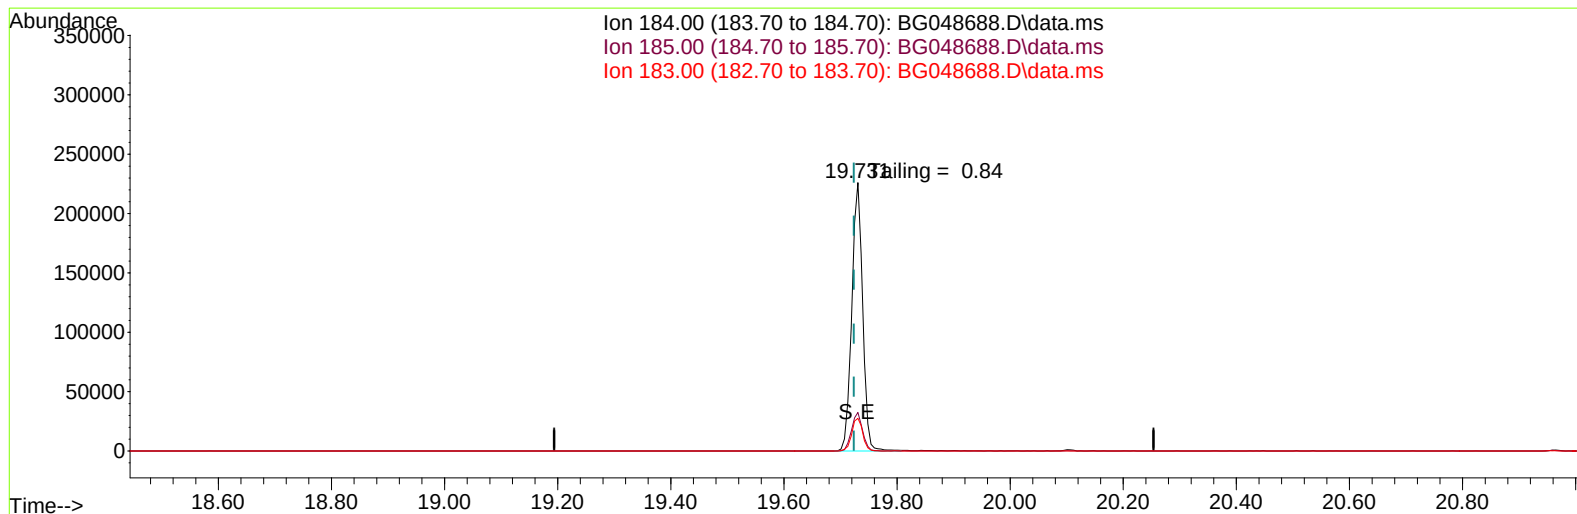

TIC: BG048688.D\data.ms

(77) Benzidine

19.731min (+ 0.007) 206428.49 ng

response 302715

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.41
183.00	11.70	12.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/14/2021	BNA_G	BG048688.D
Compound Name	Response	Retention Time
DDT	153215	20.965
DDD	244	20.61
DDE	1077	20.095
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1321	154536	0.85