
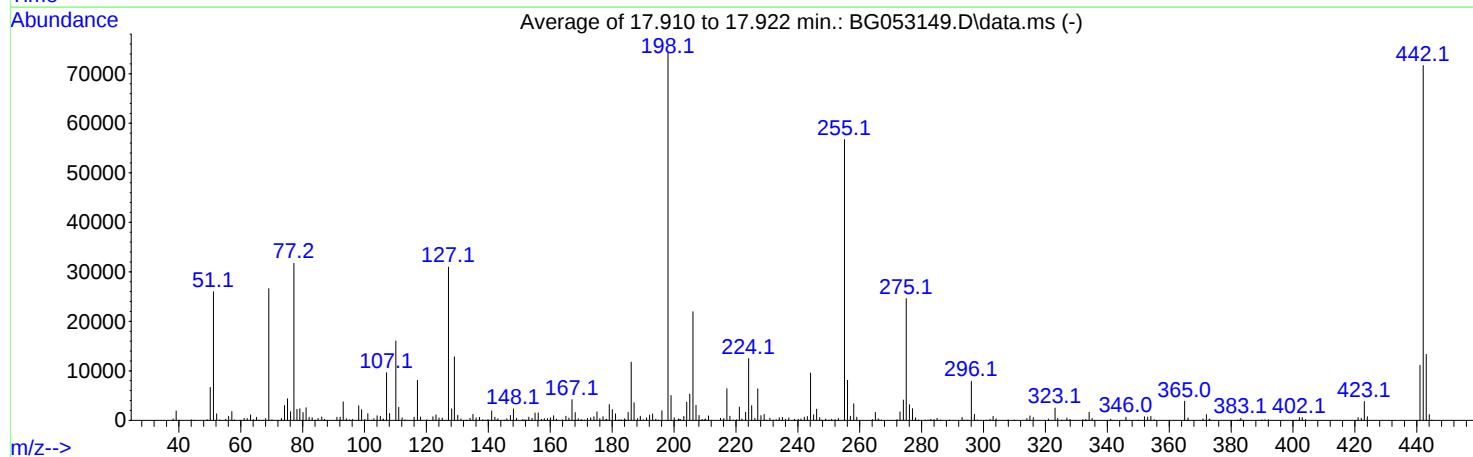


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041422\
 Data File : BG053149.D
 Acq On : 14 Apr 2022 9:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 15:31:24 2022

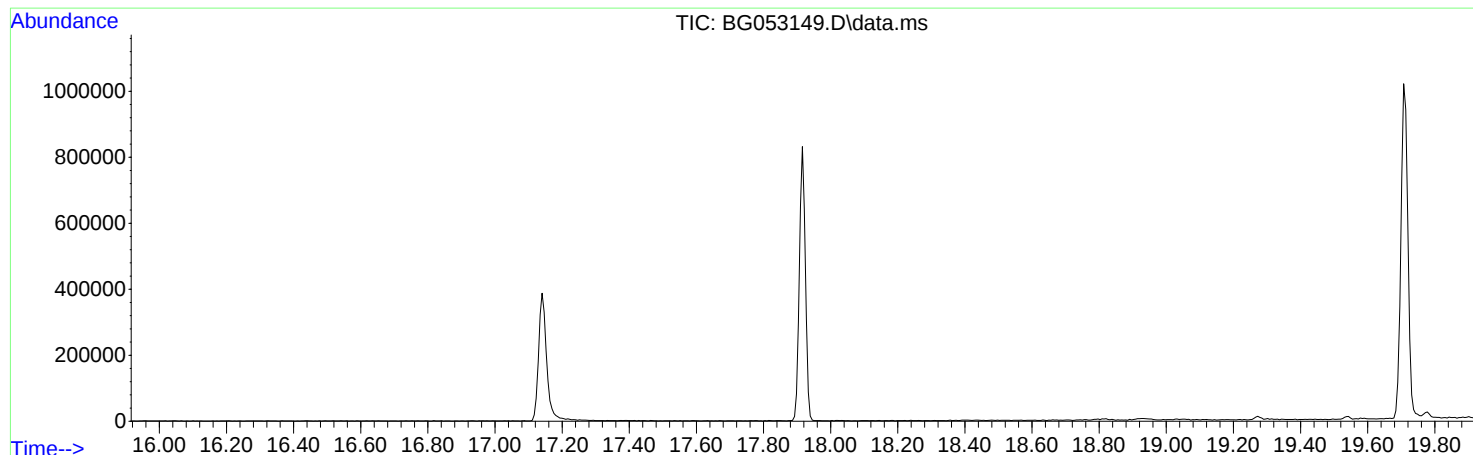




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	25987	PASS
68	69	0.00	2	1.3	346	PASS
69	198	0.00	100	35.8	26597	PASS
70	69	0.00	2	0.4	116	PASS
127	198	10	80	41.7	30971	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74299	PASS
199	198	5	9	6.8	5027	PASS
275	198	10	60	33.1	24600	PASS
365	198	1	100	5.2	3836	PASS
441	198	0.01	100	15.0	11121	PASS
442	442	50	100	100.0	71680	PASS
443	442	15	24	18.6	13319	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041422\
Data File : BG053149.D
Acq On : 14 Apr 2022 9:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 15 05:54:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

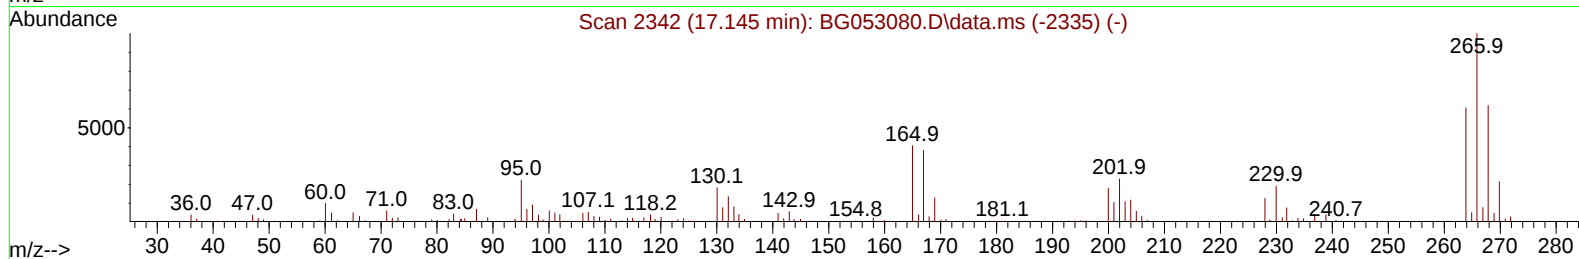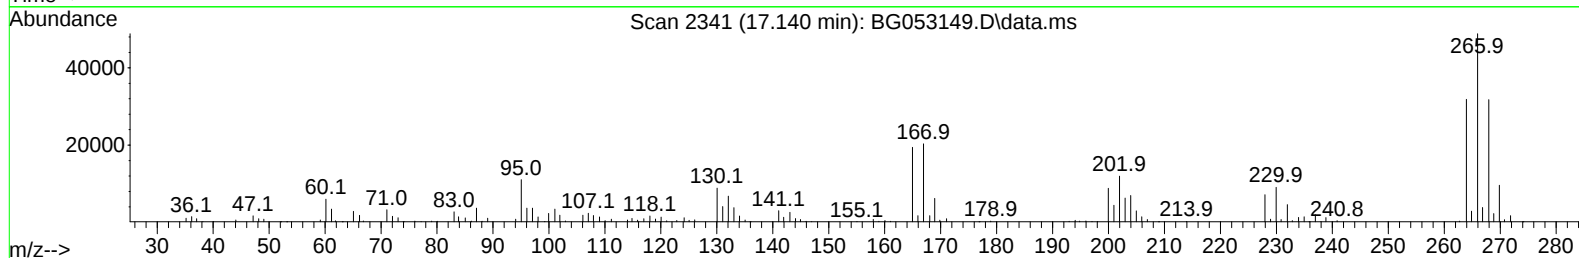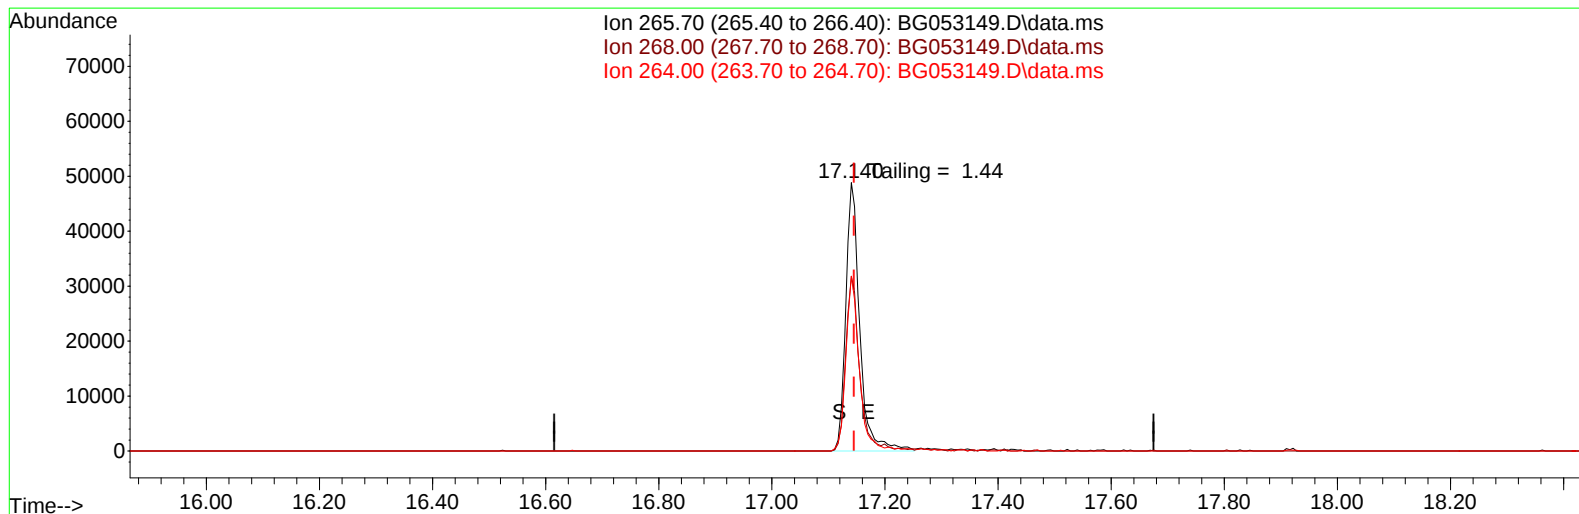

TIC: BG053149.D\data.ms

(70) Pentachlorophenol (C)

17.140min (-0.005) 20691.63 ng




response 84110

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	65.06
264.00	56.60	65.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041422\
 Data File : BG053149.D
 Acq On : 14 Apr 2022 9:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 15 05:54:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 15:31:24 2022
 Response via : Initial Calibration

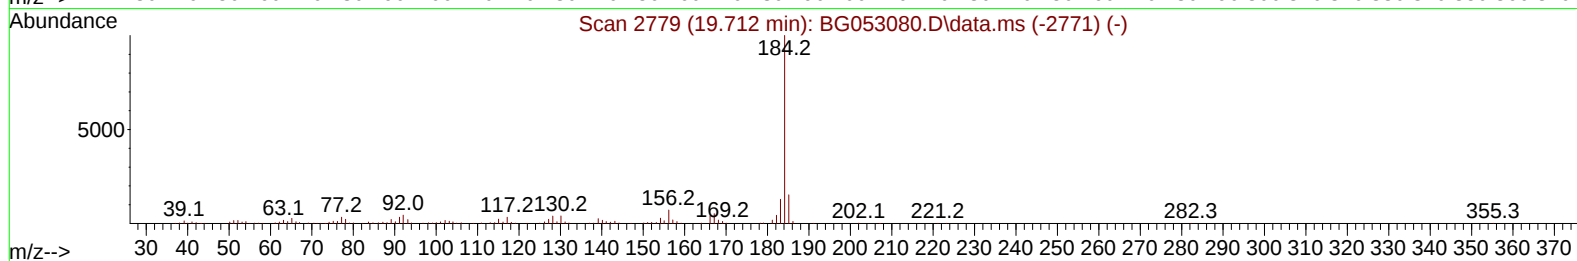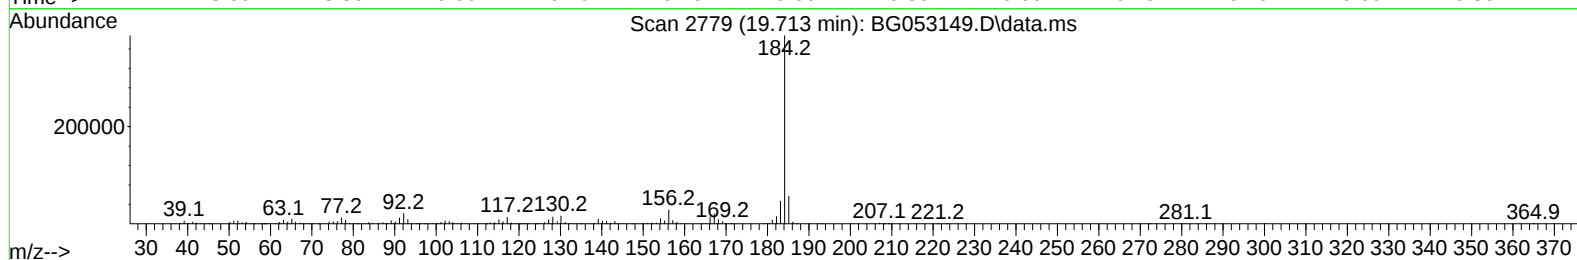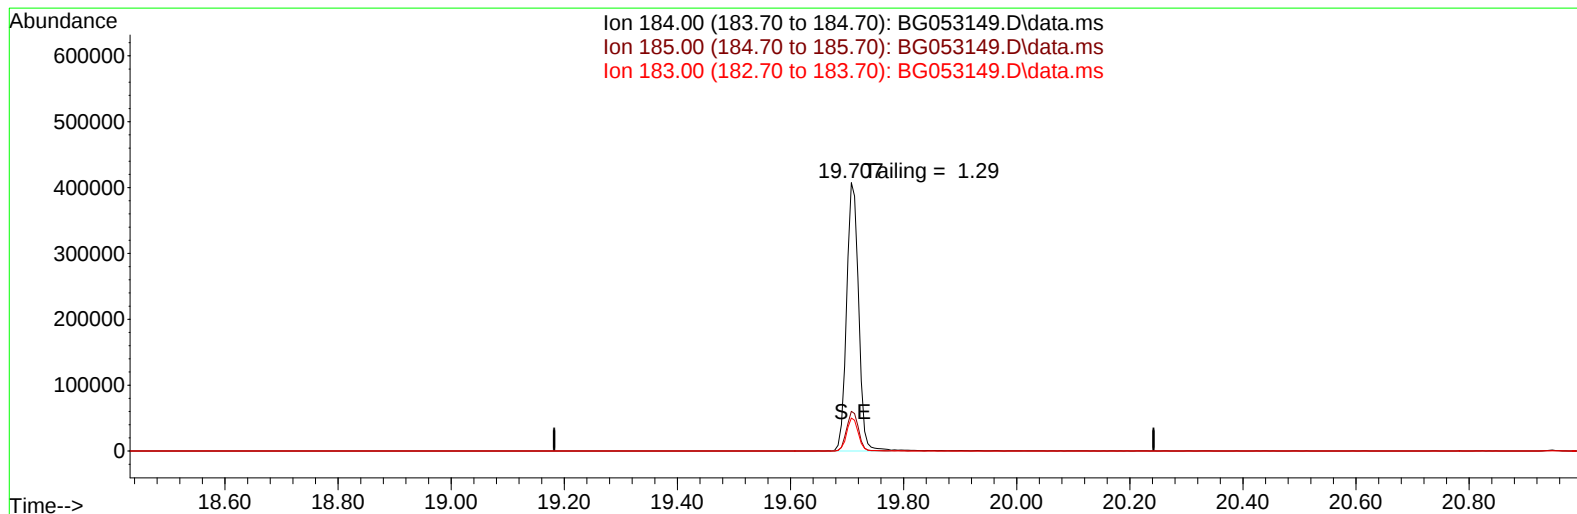

TIC: BG053149.D\data.ms

(77) Benzidine

19.712min (-19.712) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.40	0.00#
183.00	11.80	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/14/2022	BNA_G	<u>BG053149.D</u>
Compound Name	Response	Retention Time
DDT	299460	20.947
DDD	4167	20.5
DDE	331	20.001
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4498	303958	1.48

Instrument :
BNA_G
ClientSampleId :
DFTPP