


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041515\
 Data File : BG016436.D
 Acq On : 16 Apr 2015 00:15
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 14 14:00:56 2015

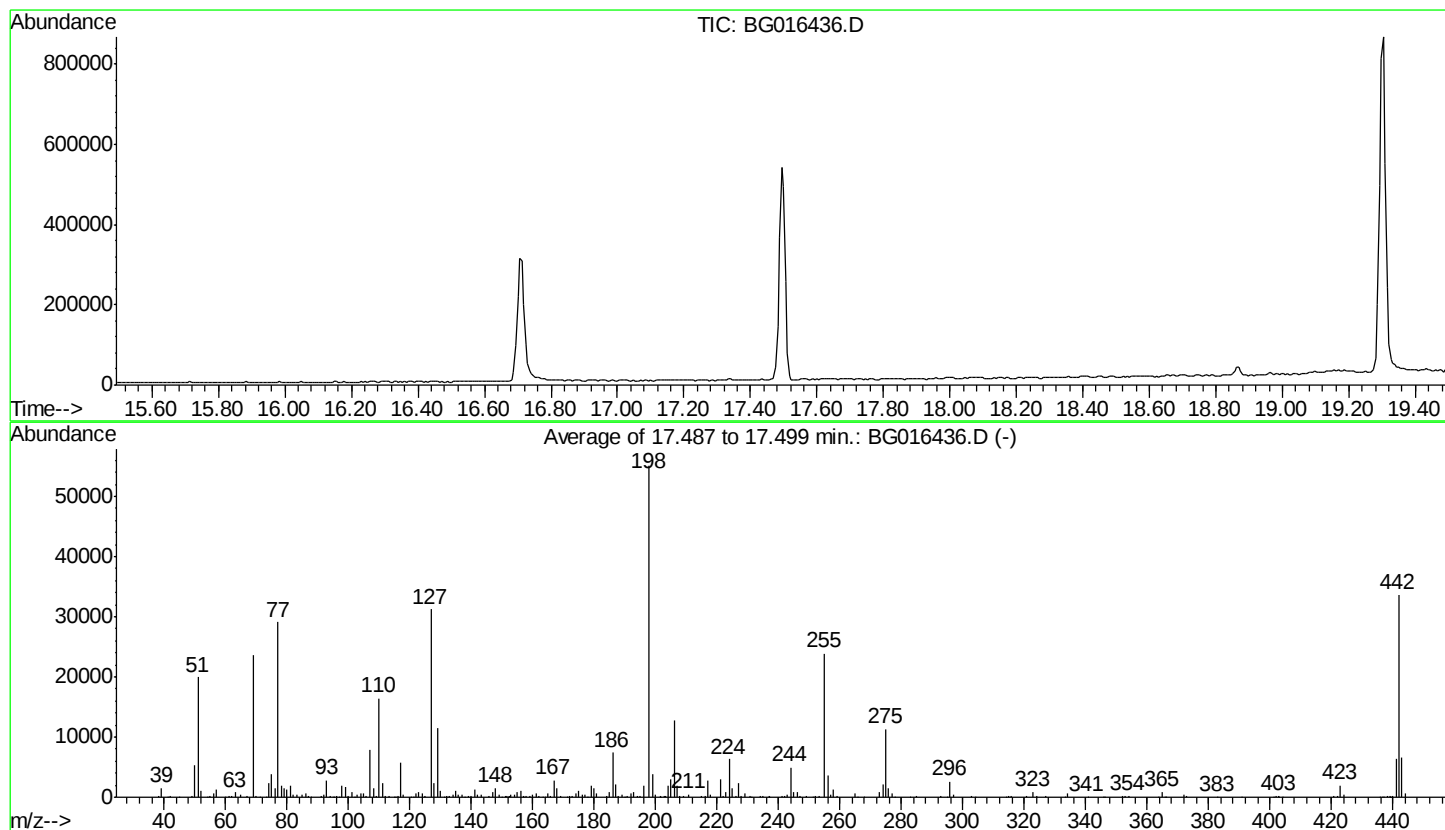

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	19972	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.9	23651	PASS
70	69	0.00	2	0.9	214	PASS
127	198	10	80	56.7	31269	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55117	PASS
199	198	5	9	6.9	3783	PASS
275	198	10	60	20.6	11330	PASS
365	198	1	100	1.7	932	PASS
441	442	0.01	24	18.8	6342	PASS
442	198	50	100	61.1	33669	PASS
443	442	15	24	19.8	6673	PASS