
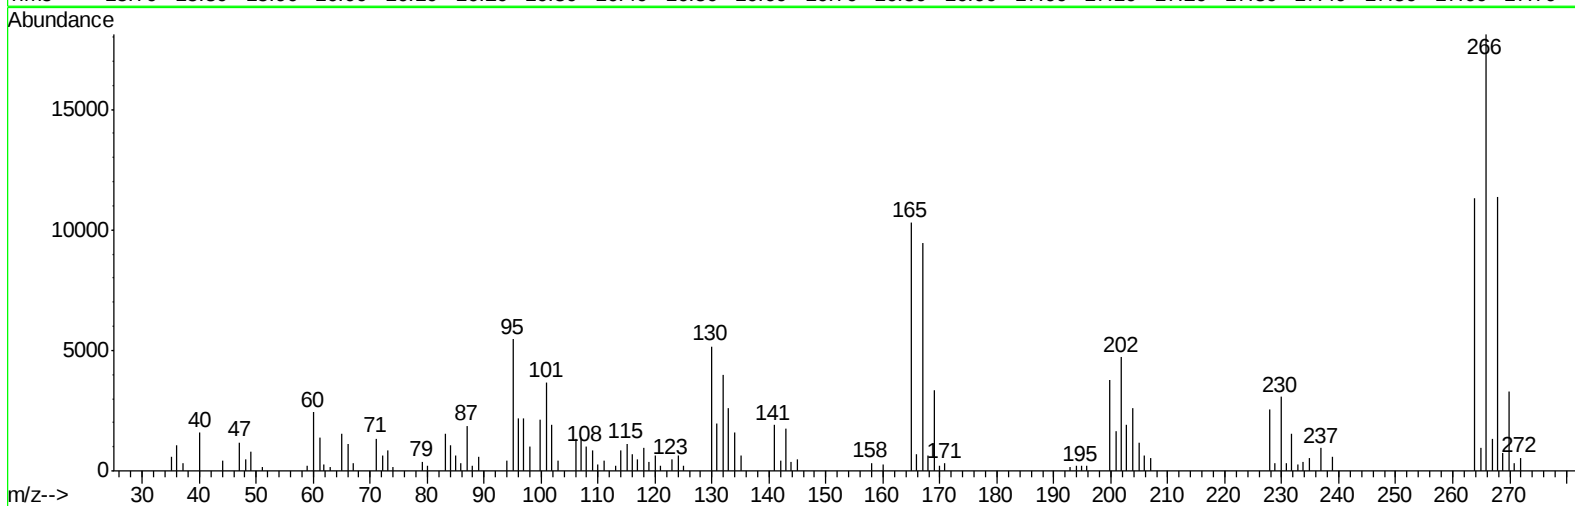


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041515\
Data File : BG016414.D
Acq On : 15 Apr 2015 10:03
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 09:09:51 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 16 04:13:21 2015
Response via : Initial Calibration

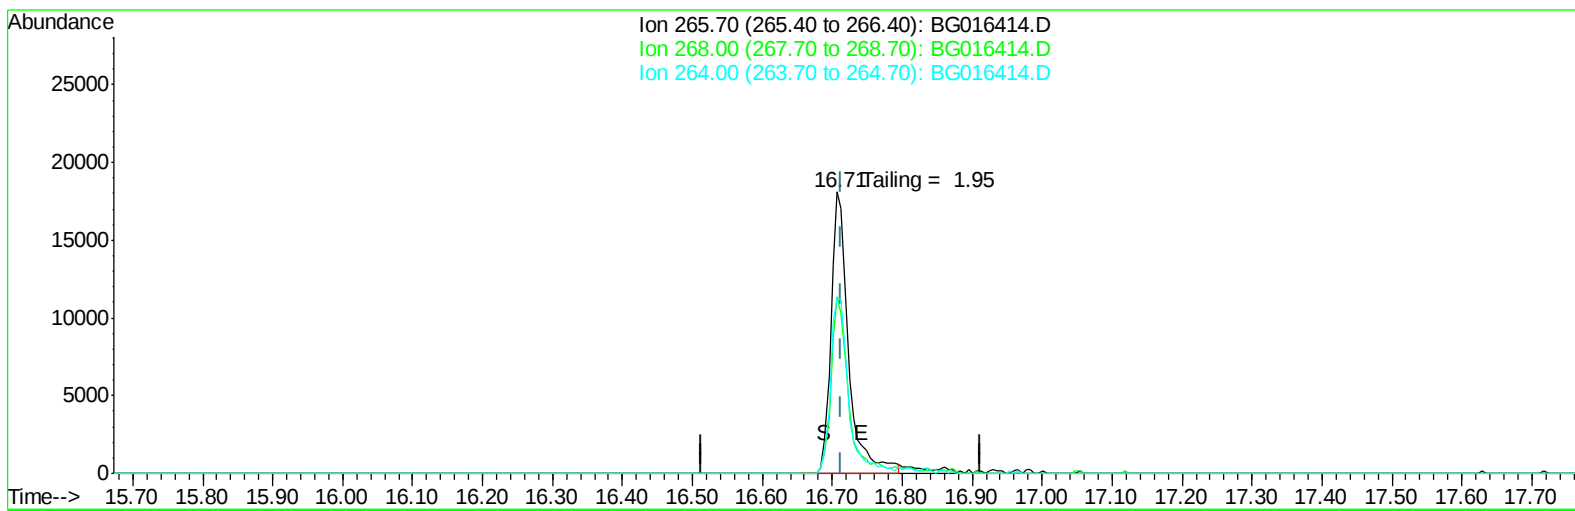

TIC: BG016414.D

(69) Pentachlorophenol (C)



16.707min (-0.006) 0.00ng

response 30116

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	62.86
264.00	66.00	62.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041515\
Data File : BG016414.D
Acq On : 15 Apr 2015 10:03
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 09:09:51 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 16 04:13:21 2015
Response via : Initial Calibration

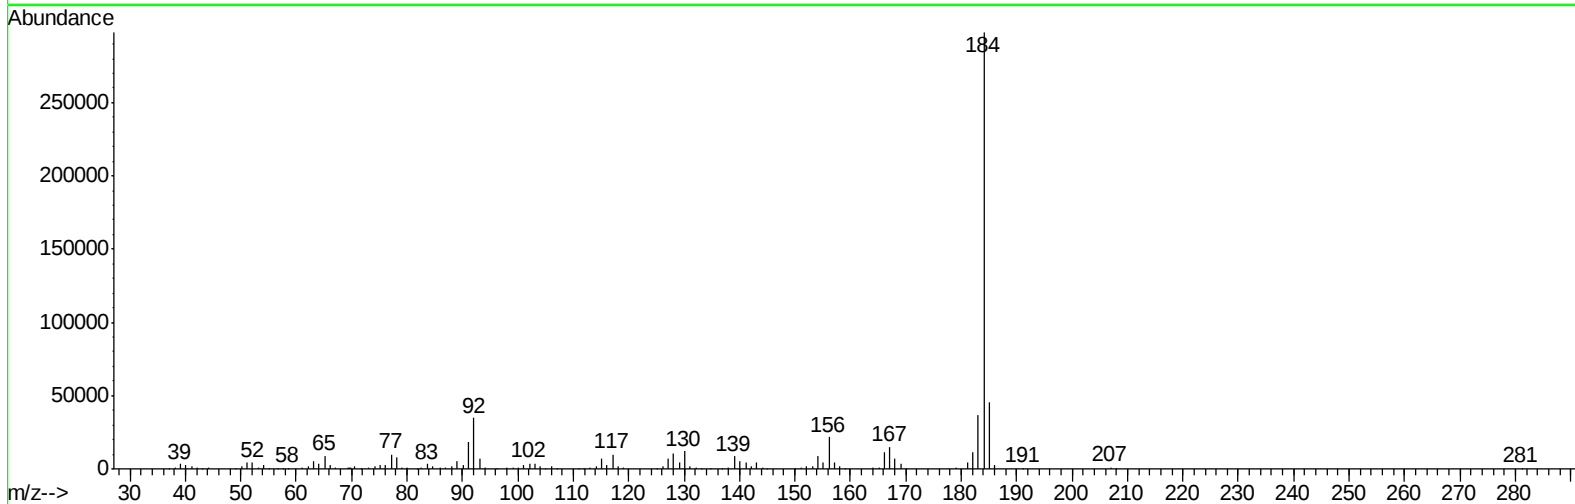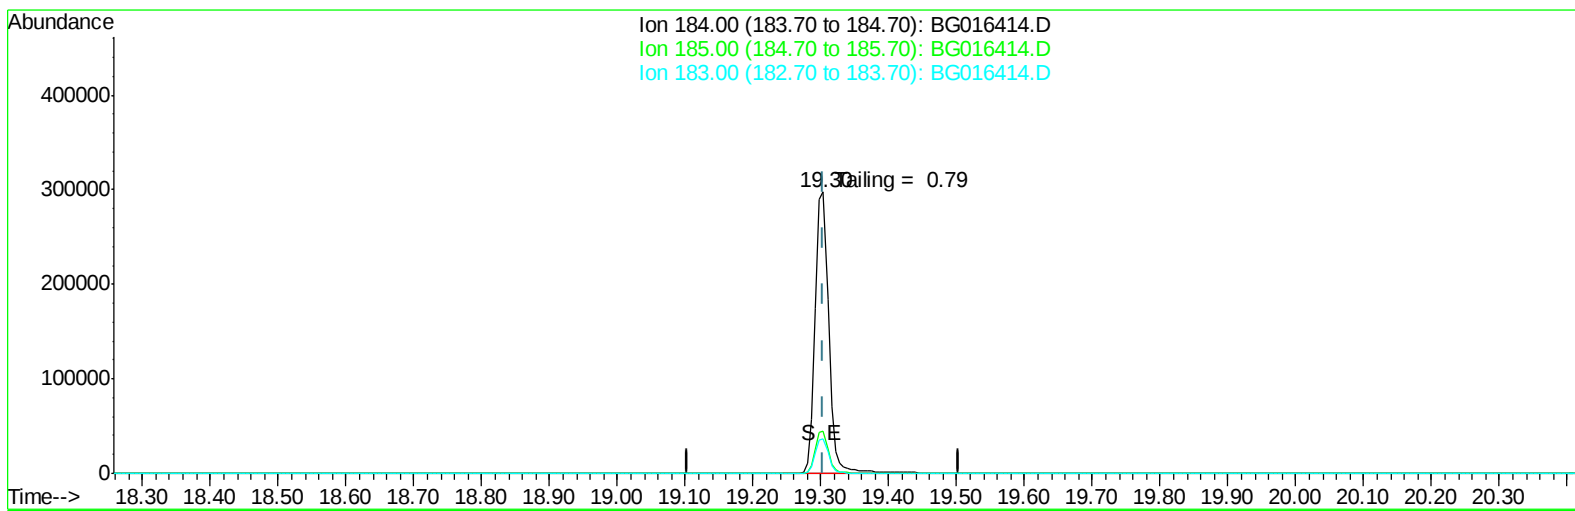

TIC: BG016414.D

(76) Benzidine

19.304min (-0.000) 0.00ng

response 409742

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.14
183.00	13.00	12.32
0.00	0.00	0.00