
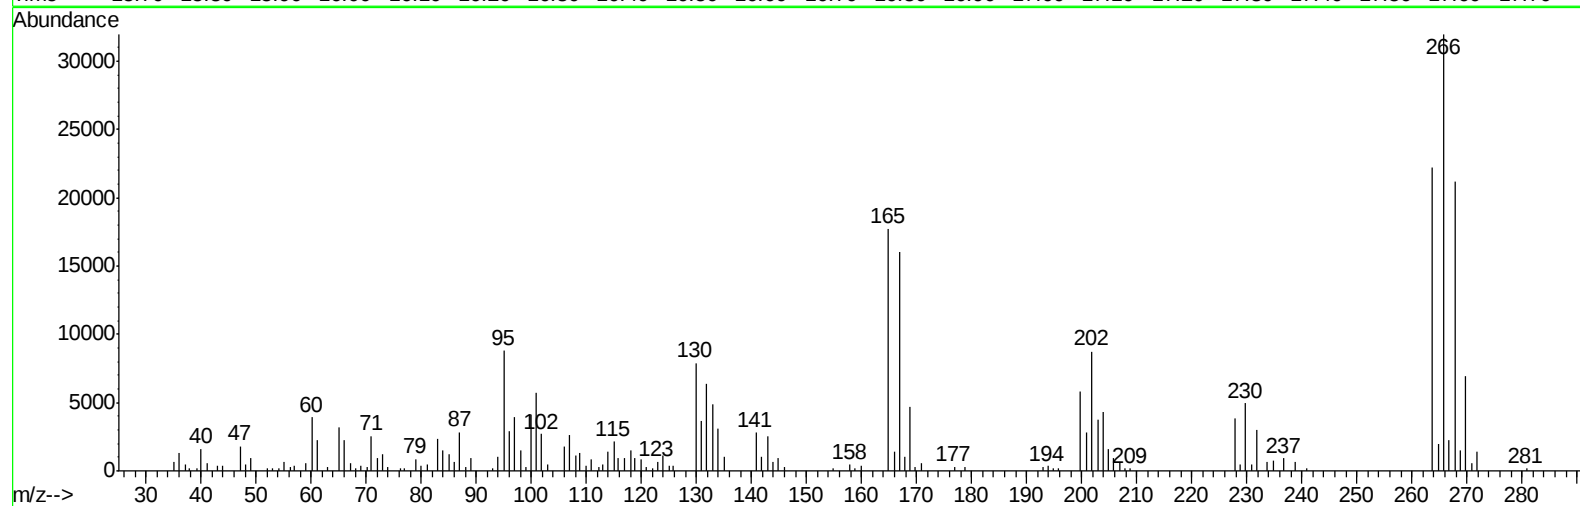


Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG041515\  
Data File : BG016436.D  
Acq On : 16 Apr 2015 00:15  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 09:12:57 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG040615.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 16 04:13:21 2015  
Response via : Initial Calibration

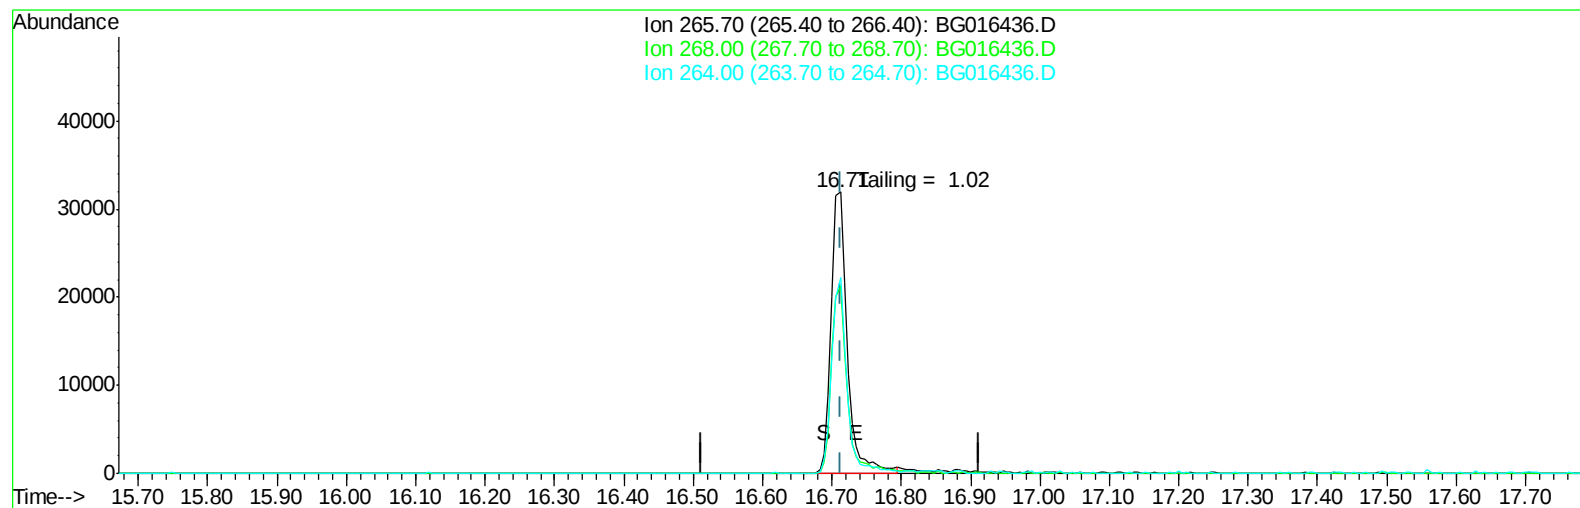

TIC: BG016436.D

(69) Pentachlorophenol (C)



16.712min (-0.001) 0.00ng

response 51184

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.60 | 66.21 |
| 264.00 | 66.00 | 69.49 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG041515\  
Data File : BG016436.D  
Acq On : 16 Apr 2015 00:15  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 09:12:57 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG040615.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 16 04:13:21 2015  
Response via : Initial Calibration

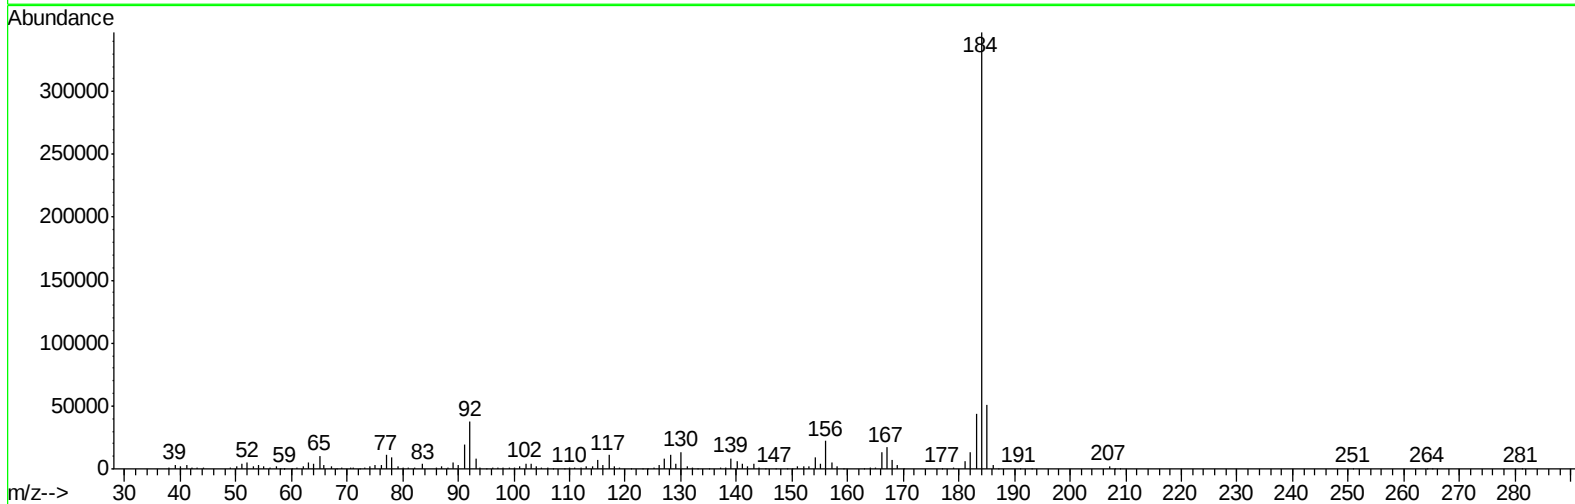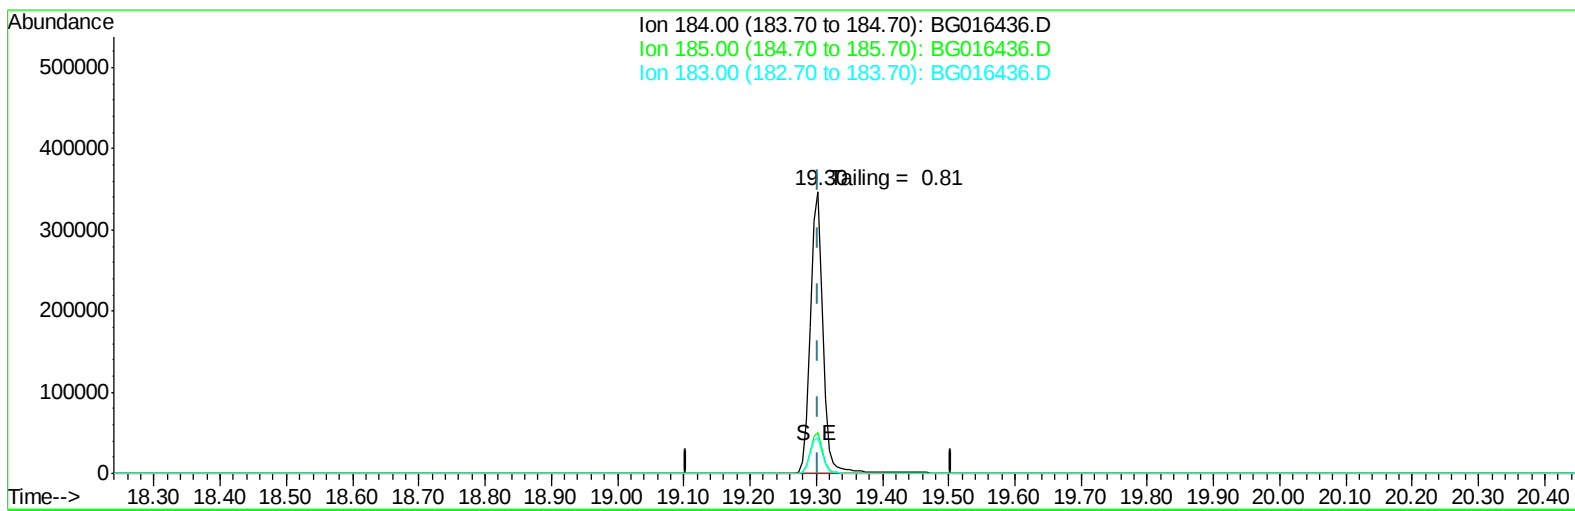

TIC: BG016436.D

(76) Benzidine

19.303min (-0.001) 0.00ng

response 464243

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.80 | 14.57 |
| 183.00 | 13.00 | 12.76 |
| 0.00   | 0.00  | 0.00  |